Serb. Astron. J. № 189 (2014), 1 - 5

Editorial

arXiv:1409.0591v1 [astro-ph.GA] 2 Sep 2014

20 CM VLA RADIO-CONTINUUM STUDY OF M 31 – IMAGES AND POINT SOURCE CATALOGUES DR2: EXTRACTION OF A SUPERNOVA REMNANT SAMPLE

T. J. Galvin, M. D. Filipović

[1] *University of Western Sydney, Locked Bag 1797, Penrith South DC, NSW 2751, Australia*
E–mail: *136525304@student.uws.edu.au, m.filipovic@uws.edu.au*

(Received: May 5, 2014; Accepted: September 2, 2014)

SUMMARY: We present Data Release 2 of the Point Source Catalogue created from a series of previously constructed radio-continuum images of M 31 at λ=20 cm (ν=1.4 GHz) from archived VLA observations. In total, we identify a collection of 916 unique discrete radio sources across the field of M 31. Comparing these detected sources to those listed by Gelfand et al. (2004) at λ=92 cm, the spectral index of 98 sources has been derived. The majority (73%) of these sources exhibit a spectral index of α <–0.6, indicating that their emission is predominantly non-thermal in nature, which is typical for background objects and Supernova Remnants (SNRs). Additionally, we investigate the presence of radio counterparts for some 156 SNRs and SNR candidates, finding a total of only 13 of these object in our images within a 5″ search area. Auxiliary optical, radio and X-ray catalogs were cross referenced highlighting a small population of SNR and SNR candidates common to multi frequency domains.

Key words. ISM: supernova remnants, Radio continuum: galaxies, Catalogs, Techniques: Image processing

1. INTRODUCTION

As a member of the Andromeda constellation, M 31 is the closest spiral galaxy to our own at a distance of $\sim$ 778 Kpc (Karachentsev et al. 2004). For this reason, it plays a significant role in galactic and extragalactic studies. A number of previous radio-continuum studies at λ=20 cm (Braun 1990a) focused on general properties of M 31, such as its structure and magnetic fields. Also, Braun (1990b) presented a list of 20 cm (5340 sources in the north-east parts of M 31. A number of other studies such as Dickel et al. (1982) estimated flux densities of M 31 supernova remnants (SNRs) and HII regions. Lee et al. (2014) identified 76 new SNRs based on Hα and [SII] images of M 31, and further confirmed a total of 80 SNR candidates from previous literature based on their selection criteria.

In this paper, we release our first revision of the data catalogue first published in Galvin et al. (2012). The original catalogue was produced from archive Very Large Array (VLA) data that was accessed and imaged from the National Radio Astronomy Observatory (NRAO) online data retrieval system at λ=20 cm. Here, we also investigate the SNR component of our sample of radio sources in the M 31.

2. DATA AND IMAGE CREATION

A collection of existing, archived radio-continuum observations at λ=20 cm with pointings centred on M 31 were obtained from the National Radio Astronomy Observatory (NRAO)[1] online data retrieval system. In total, 15 VLA projects with a variety of array configurations were selected for use in this study, as summarised in Table 1 of Galvin et al. (2012). These projects were observed between the 1^{st} of October 1983 and 27^{th} of September 1997 and are comprised of 28 individual observational runs.

The MIRIAD (Sault et al. 1995) and KARMA (Gooch 1996) software packages were used for data reduction and analysis. Initially, observations were loaded into AIPS and had their source coordinates converted from the B1950 to the J2000 reference frame. They were then exported to FITS files so that they could be loaded into the MIRIAD software package, which was then used to perform actual data reduction. Typical calibration, flagging and imaging procedures were then carried out (Sault et al. 1995). For more information on data analysis and image creation, as well as the complete set of final images used for source identification, see Galvin et al. (2012), Galvin et al. (2014), O'Brien et al. (2013) and Payne et al. (2004a).

3. RESULTS

Using the images produced in Galvin et al. (2012), we re-evaluate the unique source catalogue produced through that work. Table 1 lists all sources and the images in which they were found. Using a $2''$ search radius, this source catalogue from Galvin et al. (2012) was internally cross referenced to identify sources which were found in more then one image. In such cases, the collection of sources was given an unique group identification number. For each of these groups, an average flux and associated error was calculated based on the individual measurements of each source in that particular group. In total, 916 unique sources were identified, and of which 109 were found in at least two images.

In Fig. 1 we present the distribution of flux densities of all unique point sources. For unique sources found in more then one image (a group), that groups average flux was used. Of the total 916 unique sources, 882 ($\sim$96%) are with flux density that is below 50 mJy. From Fig. 1 we estimate that our completeness level is $\sim$2 mJy.

In Fig. 2 we show the distribution of the average flux errors of each group (109 in total). The majority of source groups (70 out of 109) have errors which are less then 30%. Of the 109 source groups, 17 have an error that is greater then 50%, possibly indicating a population of transient sources in the field of M 31.

Our catalogue was then compared to Gelfand et al. (2004). They identified 405 sources at λ = 92cm though a VLA survey conducted in an A type configuration. Their catalogue also focused predominately on compact radio sources, as the longer baselines of the A type configuration resolved out most of the extended emission. Using a $5''$ tolerance, a total of 98 sources were found to be common between both catalogues. We estimate a spectral index ($S_\nu \propto \nu^\alpha$), for these 98 sources using flux density measurements at λ=20 and 92 cm. In the event where a λ=92 cm source was matched to a group of sources from this study (ie. a source found in more then one image), that groups average flux was used in the derivation of that sources spectral index. The distribution of these spectral indices is presented in Fig. 3. These sources exhibit a predominately negative spectral index, indicating a significant population of background sources and/or SNRs in M 31 field.

4. SNRs IN THE M 31

Magnier et al. (1995) presented a comprehensive study of optically identified SNR and SNR candidates in the field of M 31. Despite relatively poor seeing conditions ($> 2''$), short exposure times and imaging only a portion of M 31's complete field, a total of 179 SNR and SNR candidates were identified. An additional 55 SNR and SNR candidates were also included in Magnier et al. (1995) from earlier work by Dodorico et al. (1980), Blair et al. (1981) and Braun and Walterbos (1993). These 234 SNR and SNR candidates were reviewed individually by Lee et al. (2014). Of the 239 SNR candidates presented by Magnier et al. (1995), 154 were discounted by Lee et al. (2014) using their SNR selection criteria.

We compared our radio-continuum catalogue to Lee et al. (2014), who used Hα and [SII] images of M 31 from the Local Group Survey (LGS; Massey et al. 2006) to identify SNR candidates. Using a search criteria of S[II]/Hα > 0.4, morphology and absence of blue stars, they identified a total of 156 SNRs and SNR candidates. Of these 156, some 80 had been listed in previous studies. We searched for these 156 objects in our own catalogue using a $5''$ search radius. A total of 13 optical SNR candidates from Lee et al. (2014) were found to have radio counter-parts. Some 3 of these 13 were also detected in Gelfand et al. (2004) listed sources. These three sources, J004102+410427, J004339+412653 and J004047+405525, have spectral indices of –0.87, –0.75 and –0.31 respectively. Two SNRs with steeper spectrum are indicative of younger SNR age. Although the relatively steep spectral index of J004102+410427 is more indicative of background galaxy, this source is likely to be intrinsic to M 31 given that it lies on the ring of diffuse emission surrounding the galaxy. We also compared positions from our radio-continuum catalogue presented here and Lee et al. (2014) and found no

[1] https://archive.nrao.edu/archive/e2earchivex.jsp

significant discrepancy (see Fig. 4). The standard deviations for ΔRA and ΔDec of these 13 sources in common are $1\farcs4$ and $1\farcs3$ respectively, and have been marked in Table 2 with a * (also noted in the tables caption).

In Fig. 5 we present a radio-continuum image of M 31 that was produced in Galvin et al. (2012) overlaid with the positions of 156 SNRs and SNR candidates identified by Lee et al. (2014). The red circle represents an SNR that had been previously identified through earlier studies, while the blue cross represents new SNRs identified by Lee et al. (2014). We see a large portion of SNRs fall on, or nearby, the ring of emission which surrounds the galaxy. The spatial distribution of these SNR candidates and their coincidence with the ring of diffuse emission implies that there is a higher rate of star formation in the outer arms of the galaxy then in its central region. Sources common between our study and Lee et al. (2014) have been marked with a purple star.

We also compared our radio-continuum catalogue with Dickel et al. (1982) who observed 10 SNRs in the field of M 31 at λ=20 cm. Of these 10 SNRs, 7 were detected in our VLA images. Once cross-referenced with our own catalogue, we find the 4 strongest detected SNRs listed in Dickel et al. (1982) were present in our own images. These four common sources are J004047+405526, J004513+413616, J004135+410657 and J004513+413616 (Group Identification Number of 92) and note that their fluxes are in good agreement. The other three detected SNRs from Dickel et al. (1982) are below our detection limit.

Using existing optical, radio and X-ray catalogues we investigate the SNR population of M 31. A radio-continuum catalogue (ν=1465 MHz) comprised of 58 SNR and SNR candidates was presented by Braun and Walterbos (1993). Of these 58 sources, 24 had a signal to noise ratio above 5σ and were included for use in this study. Comparing our catalogue to the 24 Braun and Walterbos (1993) SNRs, we find that there are 8 matches within a $5''$ search radius. Of the remaining unmatched 16 SNRs some 14 have associated extended emission structure in our images. In Fig. 6 we present a radio-continuum image of M 31 that was produced in Galvin et al. (20120) overlaid with the positions of the 24 Braun and Walterbos (1993) sources with a signal to noise ration above 5σ. The red circles represent sources common to both, our and Braun and Walterbos (1993) study, while the purple crosses represent sources from Braun and Walterbos (1993) that unmatched when compared to our work.

Additionally, 47 X-ray SNR and SNR candidates were identified by Sasaki et al. (2012) using the *XMM-Newton* telescope. Comparing Sasaki et al. (2012) to our catalogue, we find at total of 11 sources in common.

Fig. 7 is a Venn diagram showing the source intersection of these three catalogues using a search radius of $5''$. It is not surprising that there is only <10% (13 out of 156) coincidences between optical SNRs and SNR candidates and their potential radio counterparts. While in the Magellanic Clouds the ratio between known radio and optical SNRs are $\sim$ 90% (Bozzetto et al. 2014 in prep.; Haberl et al. 2012; Filipović et al 2008, 2005; Payne et al. 2008, 2007, 2004b) in other nearby galaxies this ratio is in order of 10%. For example: NGC 300 ratio is 14% (Millar et al. 2011, 2012), NGC 7793 ratio is 23% (Galvin at al. 2014 in prep.; Pannuti et al. 2011) and NGC 55 ratio is 10% (O'Brien et al. 2013). This may indicate that either our present searches for SNRs in the M 31 are not complete and/or biased towards the optical detection implying optical criteria to be bit more sensitive.

At the same time, we point out that the various density environments in which SNRs are expanding also have an effect on their detections. While radio observations are biased towards the detections of SNRs embedded in higher density environments, optical searches are more sensitive toward SNRs in low density mediums (see Pannuti et al. 2000). Coupling this with the larger distances to external galaxies (and therefore poorer resolution and sensitivity) our searches for external SNRs are at the moment introducing significant selection effects. Therefore, any comparison of SNRs in external galaxies should be taken with great caution.

CONCLUSION

We present version two of our point source catalogue of M 31 that was created using archived VLA data at λ=20 cm. In total, 916 unique sources were identified across 15 various VLA projects. Of these 916 sources, 109 of them were found in at least two different images. The spectral index for 98 sources was derived by comparing our catalogue to Gelfand et al. (2004), who lists sources at λ=92 cm. Also, we compared the optical SNR search results of Lee et al. (2014) to our radio-continuum maps of M 31, showing 13 SNRs and SNR candidates in common to two surveys to reside on the ring of diffuse emission surrounding the galaxy. Auxiliary optical, radio and X-ray catalogs were cross referenced highlighting a small population of SNR and SNR candidates common to multi frequency domains.

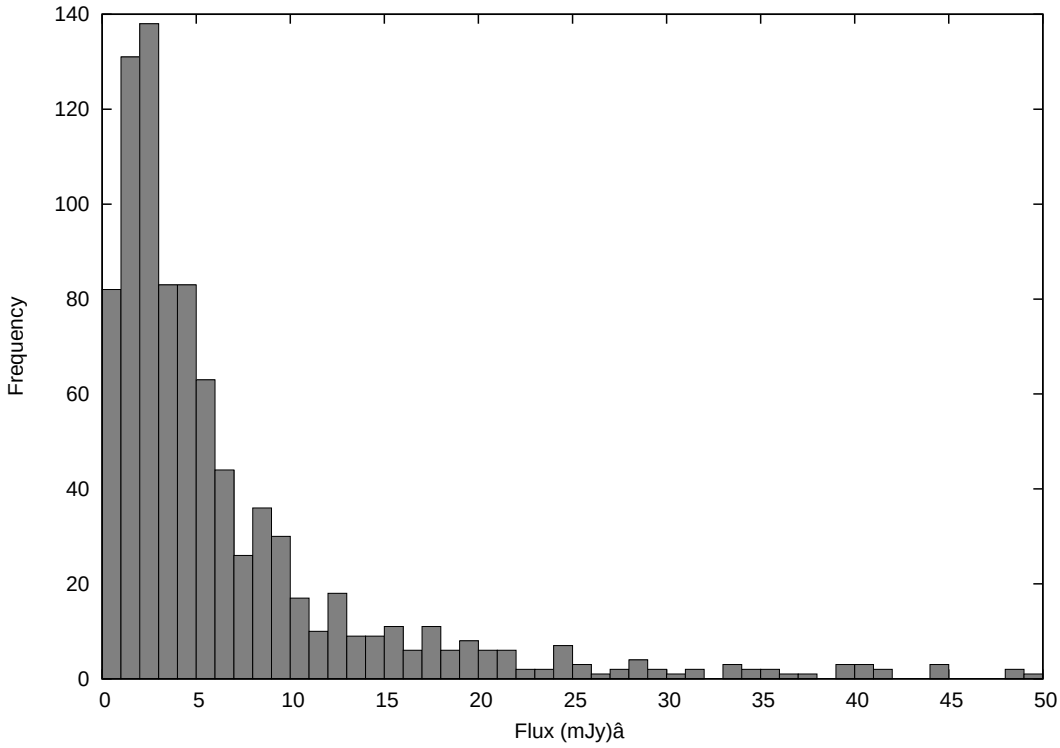

Fig. 1. *The distribution of flux densities for 916 radio sources found in M 31. 34 sources, whose flux density was above 50 mJy, have been excluded from this graph.*

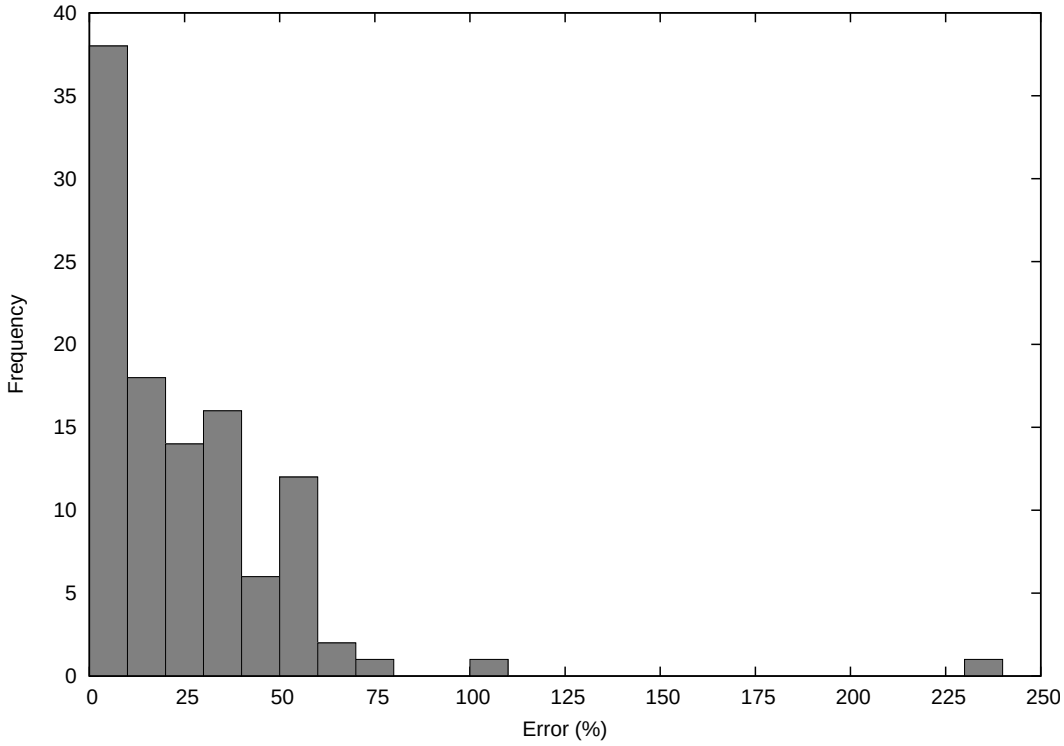

Fig. 2. *The distribution of errors for the average flux density in each group of unique sources.*

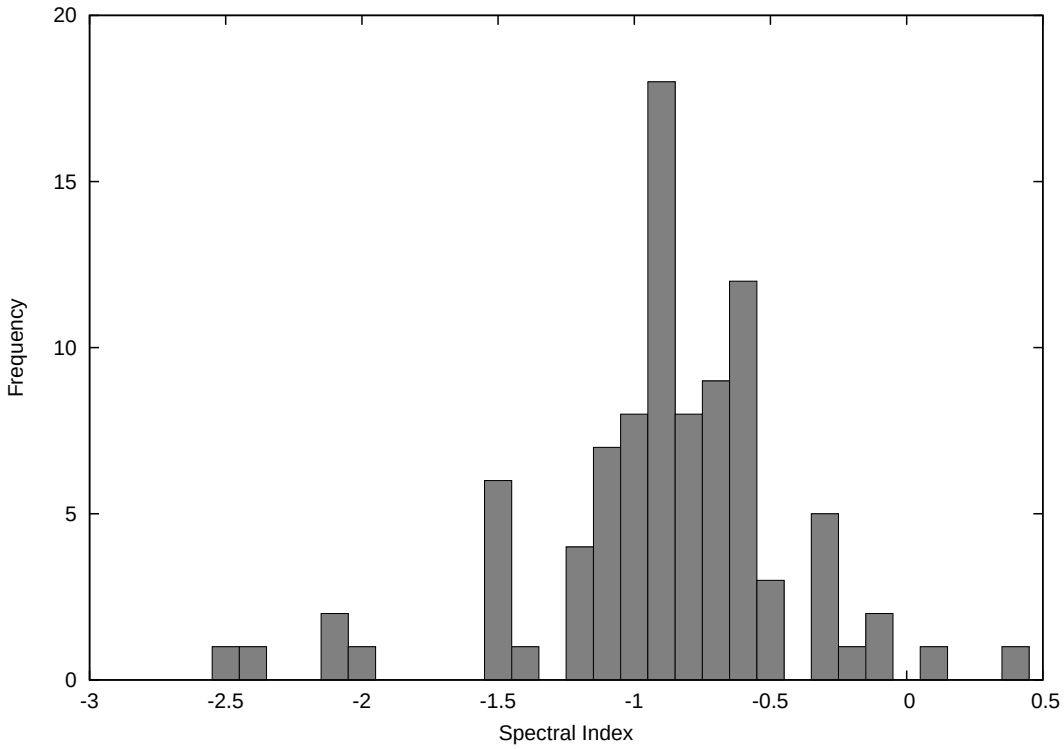

Fig. 3. *Spectral index distribution of 98 point sources in the field of M 31.*

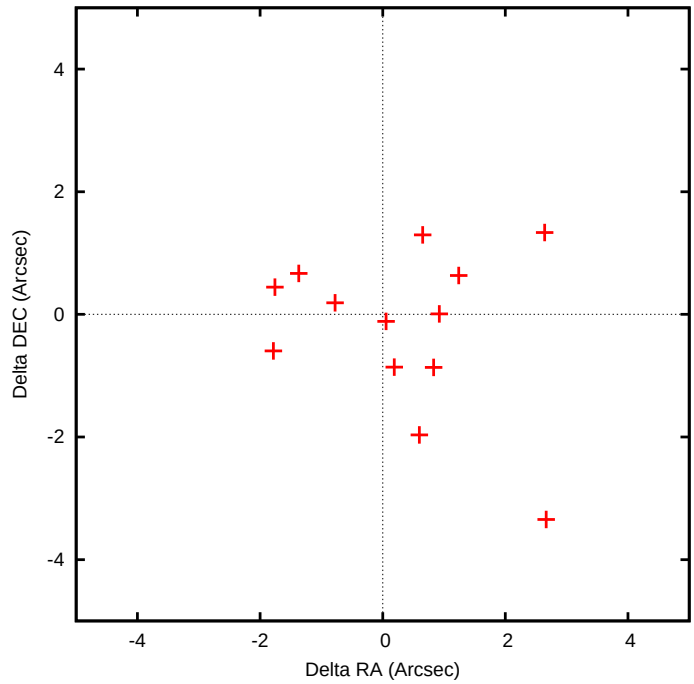

Fig. 4. *RA and Dec offsets of 13 SNRs and SNR candidates common between this study and Lee et al.*

(2014). The standard deviations for ΔRA and ΔDec are 1.4″ and 1.3″ respectively.

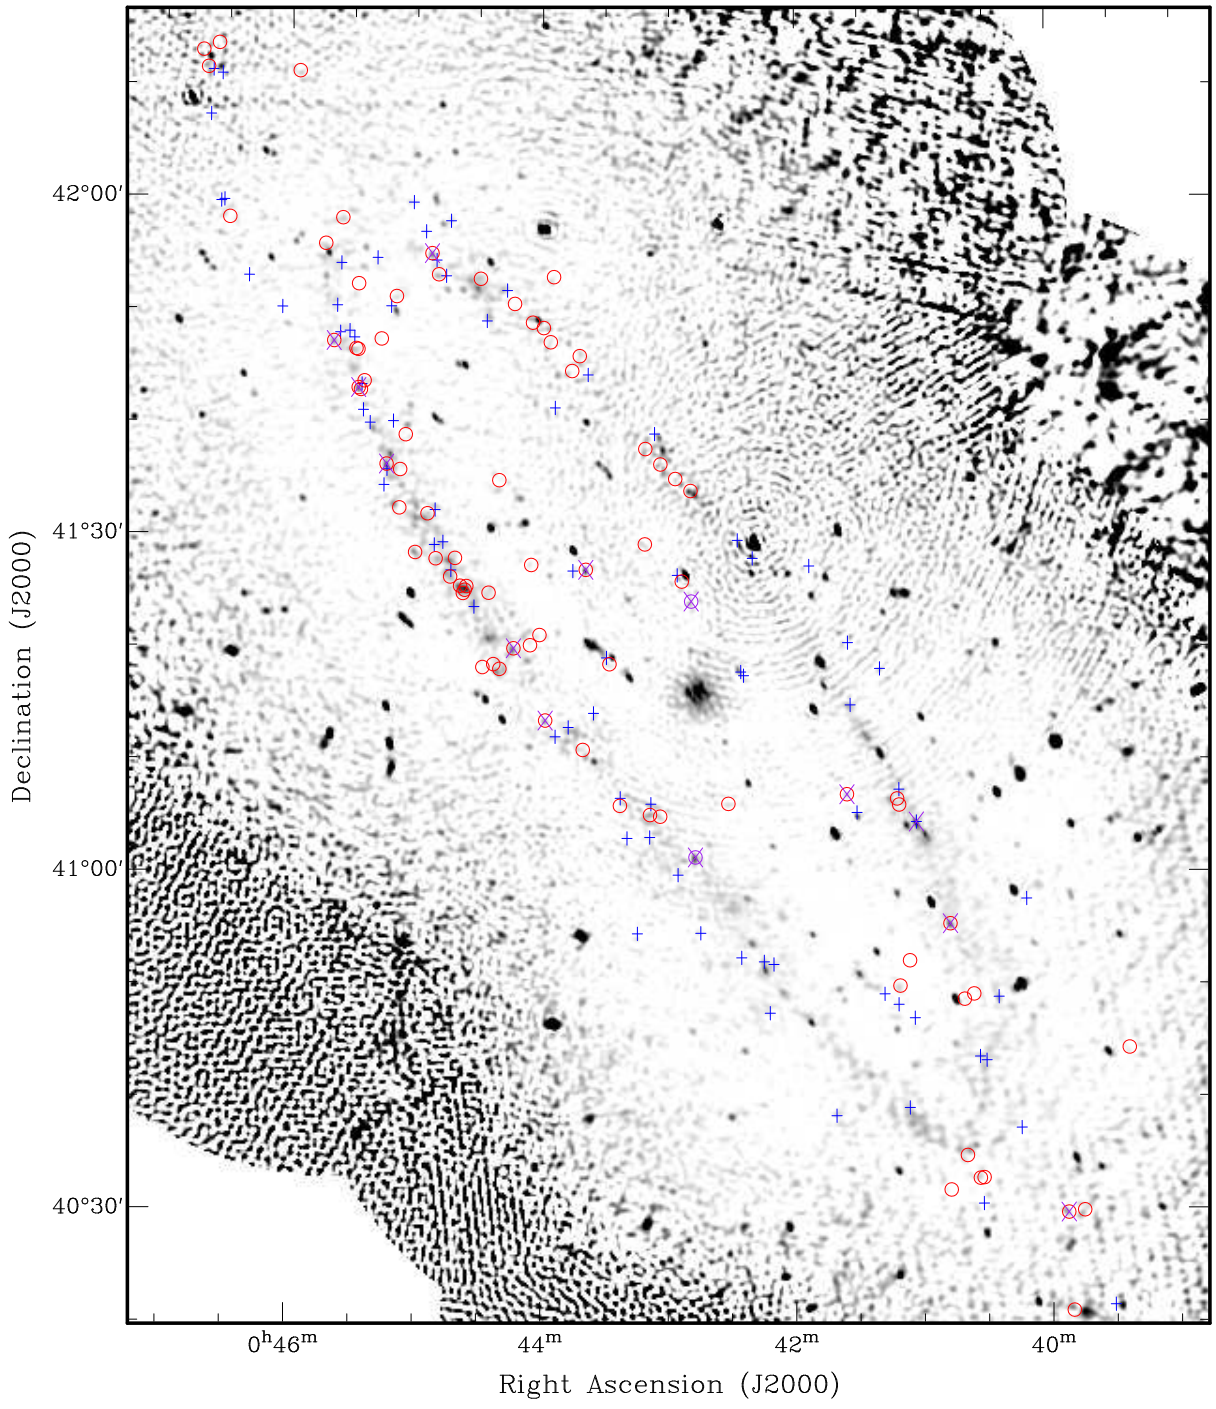

Fig. 5. *A radio-continuum image of M 31 from Galvin et al. (2012) overlaid with the positions of SNRs identified by Lee et al. (2014). The red circle represents an all previously identified SNRs that were presented in Lee et al. (2014), while the blue cross represents new SNR candidates identified by Lee et al. (2014). The purple stars highlight sources common both to our study and those presented by Lee et al. (2014).*

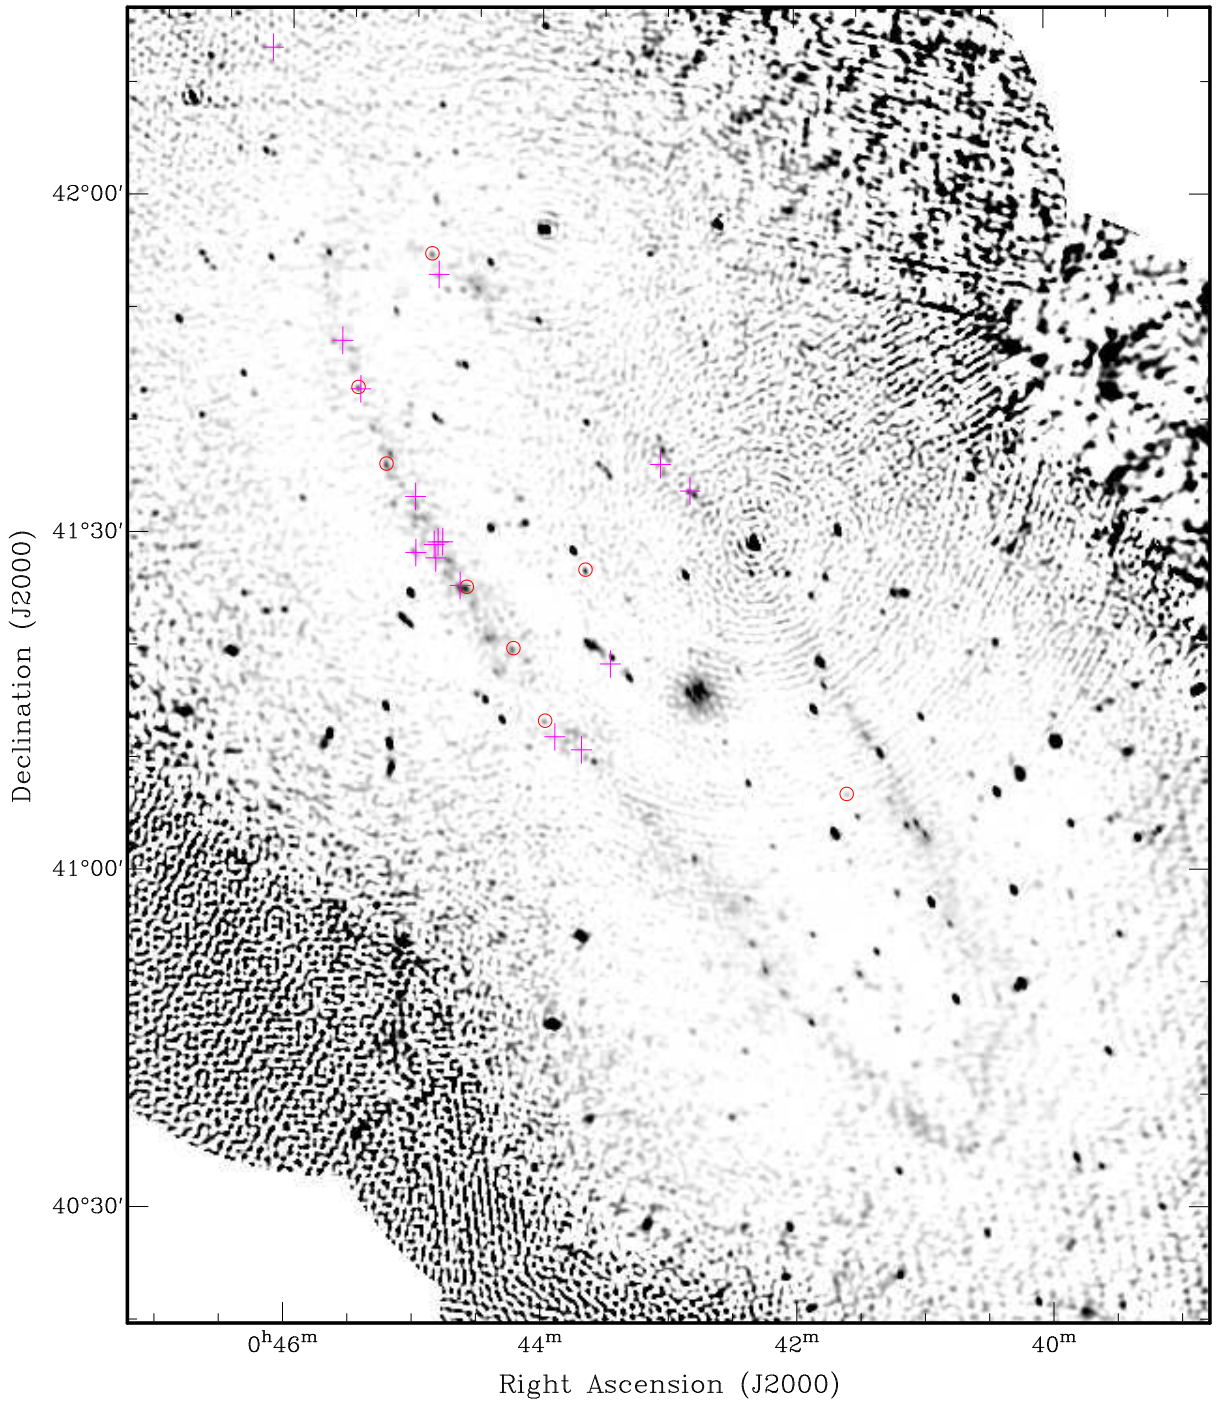

Fig. 6. *A radio-continuum image of M 31 from Galvin et al. (2012) overlaid with the positions of SNRs identified by by Braun and Walterbos (1993). The red circle represents sources common to both our study and those listed in Braun and Walterbos (1993), while the purple crosses represent sources in Braun and Walterbos (1993) which did not have a corresponding source in our study.*

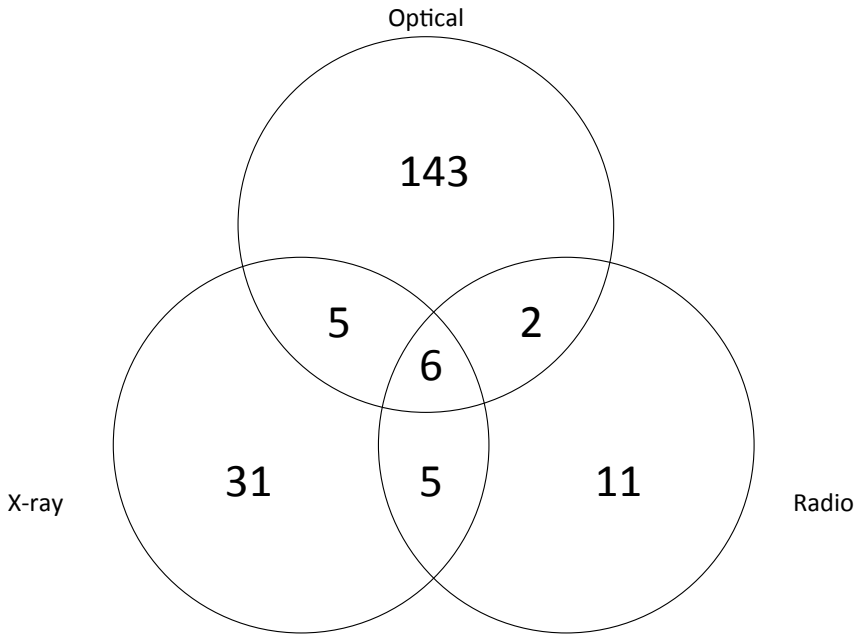

Fig. 7. *Venn Diagram showing the intersection of sources from optical (Lee at al. (2014)), radio (Braun and Walterbos (1993)) and X-ray (Sasaki et al. (2012)) catalogues from SNR and SNR candidates sources in the field of M 31.*

Table 1: A summary of all flux density measurements from sources detected in imaged projects. Column 1 is the name of the source, Column 2 and Column 3 are the RA and Dec positions (J2000) of each detected source, and Column 4 is the project in which the source was found. Sources common to multiple project have been assigned a Group ID value, listed in Column 5. The size of each group is listed in Column 6. For each group a mean flux and associated error was calculated and listed in Columns 7 and 8. Columns 9 and 10 are from Gelfand et al. (2004). Column 11 is the spectral index of either Column 4 or Column 8 and Column 10. A source name marked with * indicates that it has an optical counterpart marked as an SNR candidate by Lee et al. (2014).

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J003645+404524	00:36:45.82	+40:45:24.40	7.08	AC0308-3							
J003651+404452	00:36:51.36	+40:44:52.40	4.81	AC0308-3							
J003724+403821	00:37:24.96	+40:38:21.30	2.61	AC0308-3							
J003730+401239	00:37:30.21	+40:12:39.10	4.95	AC0308-3							
J003745+402513	00:37:45.61	+40:25:13.50	22.56	AC0308-3							
J003807+405252	00:38:07.88	+40:52:52.90	3.04	AC0308-3					11.16	0.67	-0.85
J003813+403100	00:38:13.13	+40:31:00.80	5.89	AC0308-3							
J003814+403425	00:38:14.44	+40:34:25.70	6.53	AC0308-3							
J003817+405110	00:38:17.55	+40:51:10.90	2.85	AC0308-3							
J003817+410220	00:38:17.91	+41:02:20.30	5.18	AC0308-3							
J003818+410040	00:38:18.16	+41:00:40.30	5.01	AC0308-3							
J003819+405414	00:38:19.60	+40:54:14.40	12.46	AC0308-3							
J003821+404136	00:38:21.04	+40:41:36.70	4.59	AB0437-b							
J003821+411916	00:38:21.55	+41:19:16.20	5.13	AC0308-3							
J003825+413704	00:38:25.63	+41:37:04.10	83.66	AC0308-3							
J003832+413433	00:38:32.35	+41:34:33.60	2.19	AC0308-3							
J003833+404956	00:38:33.37	+40:49:56.20	3.98	AC0308-3							
J003838+415149	00:38:38.95	+41:51:49.20	4.54	AC0308-3							
J003839+403300	00:38:39.00	+40:33:00.60	4.85	AB0437-b							
J003839+412611	00:38:39.00	+41:26:11.10	3.66	AC0308-3							
J003845+403326	00:38:45.20	+40:33:26.50	5.44	AC0308-3							
J003848+395206	00:38:48.51	+39:52:06.60	6.19	AC0308-3							
J003848+411606	00:38:48.75	+41:16:06.40	84.03	AB0437-a							
J003849+411608	00:38:49.05	+41:16:08.60	20.45	AC0308-3							
J003849+411606	00:38:49.59	+41:16:06.81	73.55	AH0524-a							
J003849+411601	00:38:49.66	+41:16:01.30	6.19	AM0464-a							
J003854+401636	00:38:54.51	+40:16:36.60	4.17	AC0308-3							
J003856+403210	00:38:56.74	+40:32:10.60	5.54	AC0308-3							
J003903+403051	00:39:03.17	+40:30:51.50	3.54	AC0308-3							
J003904+410822	00:39:04.30	+41:08:22.20	2.46	AB0437-a							
J003907+410346	00:39:07.94	+41:03:46.10	20.65	AB0437-a							
J003908+403007	00:39:08.25	+40:30:07.71	2.88	AB0437-b							
J003908+410338	00:39:08.28	+41:03:38.21	7.59	AB0437-a							
J003908+410335	00:39:08.39	+41:03:35.80	6.62	AB0437-b							
J003908+403009	00:39:08.78	+40:30:09.99	1.84	AM0464-a							
J003909+403010	00:39:09.25	+40:30:10.40	7.88	AC0308-3							
J003916+403629	00:39:16.37	+40:36:29.37	0.59	AM0464-a							
J003916+410440	00:39:16.51	+41:04:40.90	5.07	AC0308-3							
J003917+410258	00:39:17.98	+41:02:58.90	9.85	AB0437-b							
J003918+405513	00:39:18.13	+40:55:13.90	3.26	AC0308-3							
J003918+410301	00:39:18.15	+41:03:01.10	12.43	AB0437-a							
J003918+410257	00:39:18.16	+41:02:57.30	9.52	AC0308-3							
J003918+411636	00:39:18.45	+41:16:36.30	4.08	AC0308-3							
J003918+411634	00:39:18.88	+41:16:34.06	5.65	AB0437-a							
J003919+402206	00:39:19.50	+40:22:06.08	0.74	AM0464-a							
J003921+411404	00:39:21.24	+41:14:04.90	4.40	AC0308-3							
J003922+411040	00:39:22.15	+41:10:40.95	3.70	AH0524-a							
J003922+411038	00:39:22.16	+41:10:38.50	3.01	AM0464-a							
J003922+411040	00:39:22.43	+41:10:40.10	11.38	AB0437-a							
J003922+411500	00:39:22.87	+41:15:00.80	4.48	AC0308-3							
J003923+411045	00:39:23.05	+41:10:45.50	2.65	AC0308-3							
J003927+405429	00:39:27.28	+40:54:29.00	4.37	AB0437-a							
J003927+405423	00:39:27.43	+40:54:23.60	6.71	AC0308-3							
J003927+402123	00:39:27.61	+40:21:23.46	0.75	AM0464-a							
J003929+414607	00:39:29.72	+41:46:07.60	24.62	AC0308-3							
J003929+415456	00:39:29.75	+41:54:56.30	2.58	AC0308-3							
J003930+410440	00:39:30.87	+41:04:40.10	6.91	AB0437-a							
J003931+411502	00:39:31.09	+41:15:02.08	2.18	AB0437-a							
J003931+411511	00:39:31.41	+41:15:11.85	2.36	AH0524-a							
J003932+410440	00:39:32.22	+41:04:40.71	1.17	AH0524-a							
J003932+404402	00:39:32.71	+40:44:02.30	12.54	AC0308-3							
J003932+400837	00:39:32.83	+40:08:37.90	50.17	AC0308-3					156.98	11.37	-0.75
J003932+404403	00:39:32.95	+40:44:03.50	9.87	AB0437-b							
J003933+404401	00:39:33.02	+40:44:01.40	7.11	AM0464-a							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J003933+404406	00:39:33.06	+40:44:06.40	8.14	AB0437-a							
J003933+400848	00:39:33.12	+40:08:48.00	6.73	AM0464-a							
J003933+404405	00:39:33.35	+40:44:05.34	4.16	AH0221-a							
J003935+411430	00:39:35.87	+41:14:30.69	3.84	AB0437-a							
J003936+411426	00:39:36.29	+41:14:26.10	4.78	AC0308-1							
J003936+403351	00:39:36.58	+40:33:51.00	3.91	AB0437-b							
J003938+410327	00:39:38.55	+41:03:27.90	5.31	AC0308-1							
J003940+400058	00:39:40.13	+40:00:58.00	3.66	AC0308-3							
J003943+402042	00:39:43.16	+40:20:42.20	24.52	AC0308-3							
J003947+403328	00:39:47.17	+40:33:28.36	0.50	AM0464-a							
J003947+411134	00:39:47.35	+41:11:34.80	11.62	AB0437-b							
J003948+403904	00:39:48.21	+40:39:04.10	3.39	AC0308-3							
J003948+403430	00:39:48.26	+40:34:30.60	7.70	AC0308-3							
J003948+403433	00:39:48.29	+40:34:33.91	6.08	AM0464-a					12.57	11.71	-0.48
J003948+403437	00:39:48.30	+40:34:37.40	10.19	AB0437-b							
J003949+410421	00:39:49.41	+41:04:21.22	6.32	AH0221-a					14.75	0.99	-0.56
J003949+410418	00:39:49.53	+41:04:18.20	7.95	AB0437-b							
J003949+405802	00:39:49.99	+40:58:02.21	1.92	AB0437-b							
J003950+410424	00:39:50.10	+41:04:24.00	7.68	AH0524-a							
J003950+405758	00:39:50.13	+40:57:58.30	2.29	AB0437-a							
J003950+402657	00:39:50.41	+40:26:57.10	1.80	AM0464-a							
J003950+395719	00:39:50.51	+39:57:19.60	6.80	AC0308-3							
J003952+402635	00:39:52.17	+40:26:35.90	1.97	AM0464-a							
J003952+402943*	00:39:52.53	+40:29:43.20	0.66	AM0464-a							
J003956+411134	00:39:56.37	+41:11:34.90	63.62	AB0437-b							
J003956+411138	00:39:56.77	+41:11:38.30	80.32	AH0524-a							
J003957+411138	00:39:57.13	+41:11:38.70	11.93	AC0308-1							
J003957+411356	00:39:57.31	+41:13:56.20	2.13	AB0437-a							
J003957+411358	00:39:57.59	+41:13:58.00	2.53	AH0524-a							
J003959+401349	00:39:59.14	+40:13:49.50	8.04	AM0464-a							
J003959+401343	00:39:59.49	+40:13:43.80	21.80	AC0308-3							
J004002+412634	00:40:02.34	+41:26:34.40	5.37	AC0308-1							
J004002+412205	00:40:02.86	+41:22:05.10	2.15	AB0437-a							
J004004+401417	00:40:04.43	+40:14:17.47	1.49	AM0464-a							
J004005+401613	00:40:05.06	+40:16:13.15	0.85	AM0464-a							
J004005+401605	00:40:05.32	+40:16:05.10	3.21	AC0308-3							
J004005+405854	00:40:05.36	+40:58:54.23	1.79	AB0437-a							
J004006+402147	00:40:06.20	+40:21:47.80	9.60	AC0308-3							
J004006+402148	00:40:06.40	+40:21:48.40	7.37	AM0464-a							
J004007+405346	00:40:07.63	+40:53:46.60	1.09	AB0437-a							
J004010+411825	00:40:10.88	+41:18:25.90	3.47	AC0308-1							
J004012+410840	00:40:12.28	+41:08:40.73	2.85	AH0221-a							
J004013+410839	00:40:13.28	+41:08:39.05	5.16	AH0221-a							
J004013+410840	00:40:13.43	+41:08:40.30	41.68	AB0437-b							
J004013+405008	00:40:13.63	+40:50:08.30	48.96	AB0437-a							
J004013+410841	00:40:13.67	+41:08:41.00	58.76	AH0524-a							
J004014+410841	00:40:14.02	+41:08:41.10	14.23	AC0308-1							
J004014+405017	00:40:14.20	+40:50:17.26	26.65	AH0524-a							
J004014+405002	00:40:14.42	+40:50:02.10	9.71	AC0308-1							
J004016+405826	00:40:16.36	+40:58:26.96	11.91	AH0221-a							
J004016+412224	00:40:16.84	+41:22:24.30	2.83	AB0437-a							
J004016+412853	00:40:16.92	+41:28:53.90	13.73	AC0308-3							
J004017+405829	00:40:17.10	+40:58:29.20	24.44	AH0524-a							
J004017+395508	00:40:17.24	+39:55:08.10	15.54	AC0308-3							
J004017+412840	00:40:17.86	+41:28:40.73	6.01	AH0524-a							
J004022+412046	00:40:22.74	+41:20:46.40	15.09	AC0308-3							
J004024+412926	00:40:24.13	+41:29:26.70	6.09	AC0308-3					29.01	1.41	-1.02
J004024+410712	00:40:24.36	+41:07:12.95	15.92	AH0221-a							
J004024+412029	00:40:24.57	+41:20:29.00	9.37	AB0437-a							
J004024+410713	00:40:24.78	+41:07:13.50	31.70	AH0524-a							
J004024+412029	00:40:24.84	+41:20:29.50	8.27	AH0524-a							
J004024+412919	00:40:24.88	+41:29:19.64	4.75	AH0524-a							
J004024+412023	00:40:24.96	+41:20:23.70	2.62	AM0464-a							
J004025+410712	00:40:25.33	+41:07:12.80	9.94	AC0308-1							
J004025+410718	00:40:25.71	+41:07:18.64	15.49	AB0551-a							
J004026+403601	00:40:26.27	+40:36:01.32	0.46	AM0464-a							
J004026+403618	00:40:26.54	+40:36:18.20	1.85	AB0437-a							
J004027+401544	00:40:27.94	+40:15:44.50	3.33	AC0308-3							
J004028+401546	00:40:28.09	+40:15:46.23	0.86	AM0464-a							
J004028+411758	00:40:28.66	+41:17:58.30	1.84	AB0437-a							
J004029+411804	00:40:29.22	+41:18:04.90	1.95	AH0524-a							
J004029+412128	00:40:29.33	+41:21:28.60	1.68	AB0437-a							
J004030+402758	00:40:30.35	+40:27:58.50	7.73	AB0437-b							
J004031+403911	00:40:31.98	+40:39:11.10	1.89	AB0437-a							
J004032+414821	00:40:32.65	+41:48:21.20	2.77	AC0308-3							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004032+413634	00:40:32.78	+41:36:34.90	5.30	AC0308-3							
J004032+402021	00:40:32.94	+40:20:21.80	4.70	AC0308-3							
J004034+403540	00:40:34.70	+40:35:40.54	0.85	AM0464-a							
J004035+413511	00:40:35.58	+41:35:11.10	16.02	AC0308-3					13.22	0.82	0.13
J004036+413500	00:40:36.20	+41:35:00.49	9.90	AH0524-a							
J004036+410842	00:40:36.33	+41:08:42.70	1.76	AB0437-a							
J004036+411023	00:40:36.37	+41:10:23.60	2.42	AC0308-3							
J004036+411938	00:40:36.63	+41:19:38.40	1.68	AB0437-a							
J004036+410845	00:40:36.73	+41:08:45.70	1.65	AH0524-a							
J004036+412052	00:40:36.74	+41:20:52.32	2.15	AT0149-a							
J004036+412404	00:40:36.79	+41:24:04.70	3.23	AT0149-a							
J004036+411910	00:40:36.91	+41:19:10.90	15270.00	AB0491-a							
J004037+411936	00:40:37.17	+41:19:36.50	2.49	AH0524-a							
J004037+412051	00:40:37.42	+41:20:51.49	3.78	AT0149-a							
J004037+403512	00:40:37.86	+40:35:12.40	0.49	AM0464-a							
J004041+403519	00:40:41.13	+40:35:19.70	9.58	AC0308-3							
J004041+401049	00:40:41.69	+40:10:49.10	3.57	AC0308-3							
J004043+403623	00:40:43.50	+40:36:23.80	8.20	AC0308-3							
J004043+412343	00:40:43.59	+41:23:43.02	1.80	AH0524-a							
J004043+404843	00:40:43.95	+40:48:43.30	13.15	AC0308-3							
J004044+404449	00:40:44.13	+40:44:49.32	1.16	AB0437-b							
J004044+404445	00:40:44.38	+40:44:45.19	0.52	AM0464-a							
J004044+404845	00:40:44.56	+40:48:45.30	13.30	AB0491-a							
J004044+404447	00:40:44.64	+40:44:47.30	2.07	AB0437-a							
J004044+404858	00:40:44.71	+40:48:58.81	7.75	AH0524-a							
J004044+404840	00:40:44.79	+40:48:40.90	8.44	AC0308-1							
J004046+411637	00:40:46.52	+41:16:37.03	2.26	AT0149-a							
J004046+405522	00:40:46.85	+40:55:22.85	2.17	AM0464-a							
J004047+405527	00:40:47.04	+40:55:27.80	3.01	AB0437-a							
J004047+405525*	00:40:47.11	+40:55:25.17	2.62	AH0221-a					4.19	0.42	-0.31
J004047+405532	00:40:47.36	+40:55:32.90	2.22	AH0524-a							
J004047+405526	00:40:47.38	+40:55:26.50	4.12	AB0491-a							
J004047+415006	00:40:47.71	+41:50:06.20	8.75	AC0496-a							
J004047+403721	00:40:47.73	+40:37:21.00	10.54	AC0308-3							
J004049+411226	00:40:49.05	+41:12:26.92	2.30	AT0149-a							
J004052+411738	00:40:52.10	+41:17:38.90	15.09	AC0101-a							
J004053+410643	00:40:53.11	+41:06:43.90	3.60	AC0308-3							
J004054+412632	00:40:54.52	+41:26:32.00	3.88	AT0149-a							
J004056+405727	00:40:56.06	+40:57:27.60	28.52	AH0524-a							
J004056+405719	00:40:56.18	+40:57:19.20	11.75	AC0308-1							
J004056+405734	00:40:56.81	+40:57:34.31	13.90	AB0551-a							
J004056+405405	00:40:56.86	+40:54:05.60	4.22	AC0308-1							
J004057+403617	00:40:57.02	+40:36:17.00	1.55	AB0437-a							
J004057+402157	00:40:57.16	+40:21:57.55	0.96	AM0464-a							
J004057+410256	00:40:57.28	+41:02:56.40	16.63	AC0308-3							
J004057+401834	00:40:57.33	+40:18:34.80	6.57	AC0308-1							
J004057+415438	00:40:57.96	+41:54:38.20	1.17	AC0496-a					51.32	6.98	-2.48
J004057+412133	00:40:57.97	+41:21:33.30	10.70	AC0101-a							
J004058+410323	00:40:58.17	+41:03:23.70	3.88	AB0437-b							
J004058+410320	00:40:58.64	+41:03:20.29	5.75	AB0437-a							
J004059+410320	00:40:59.02	+41:03:20.40	11.76	AB0491-a							
J004100+411350	00:41:00.38	+41:13:50.17	6.39	AB0491-a							
J004101+410407	00:41:01.59	+41:04:07.70	1.24	AH0524-a							
J004101+410808	00:41:01.84	+41:08:08.50	8.15	AC0308-1							
J004102+410412	00:41:02.86	+41:04:12.49	1.57	AB0437-a							
J004102+410427*	00:41:02.94	+41:04:27.70	2.47	AM0464-a					9.26	0.41	-0.87
J004103+410430	00:41:03.03	+41:04:30.30	2.88	AH0524-a							
J004104+404254	00:41:04.19	+40:42:54.23	1.35	AM0464-a							
J004104+404255	00:41:04.37	+40:42:55.04	0.61	AB0491-a							
J004104+403826	00:41:04.59	+40:38:26.20	2.50	AB0437-a							
J004104+410417	00:41:04.71	+41:04:17.40	17.47	AB0491-a							
J004105+410416	00:41:05.06	+41:04:16.30	12.93	AC0308-3							
J004105+414451	00:41:05.89	+41:44:51.43	1.28	AC0496-a							
J004106+410407	00:41:06.85	+41:04:07.40	3.67	AB0437-b							
J004106+410415	00:41:06.90	+41:04:15.99	2.21	AB0437-a							
J004107+410414	00:41:07.12	+41:04:14.40	3.74	AM0464-a							
J004107+410417	00:41:07.33	+41:04:17.90	3.96	AH0524-a							
J004107+412129	00:41:07.74	+41:21:29.70	6.36	AC0101-a							
J004107+412453	00:41:07.84	+41:24:53.34	11.28	AH0524-a							
J004108+412444	00:41:08.09	+41:24:44.50	13.49	AC0101-a							
J004108+412457	00:41:08.70	+41:24:57.90	18.90	AC0308-3							
J004109+403853	00:41:09.12	+40:38:53.80	3.70	AC0308-3							
J004109+412451	00:41:09.37	+41:24:51.26	0.95	AM0464-a							
J004109+412456	00:41:09.61	+41:24:56.80	27.57	AB0551-a							
J004110+412456	00:41:10.53	+41:24:56.40	16.79	AC0308-1							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004111+402412	00:41:11.13	+40:24:12.70	10.59	AM0464-a							
J004111+403327	00:41:11.18	+40:33:27.90	2.55	AC0308-3							
J004111+402419	00:41:11.44	+40:24:19.90	5.24	AC0308-1							
J004111+403331	00:41:11.46	+40:33:31.70	5.06	AB0437-b							
J004111+405813	00:41:11.73	+40:58:13.80	2.89	AB0437-a							
J004111+405812	00:41:11.88	+40:58:12.19	1.79	AM0464-a							
J004111+405816	00:41:11.95	+40:58:16.60	2.61	AH0524-a							
J004112+405812	00:41:12.06	+40:58:12.60	2.97	AB0491-a							
J004112+412458	00:41:12.10	+41:24:58.60	44.01	AB0679-a							
J004112+412458	00:41:12.32	+41:24:58.10	4.45	AB0679-b							
J004112+415643	00:41:12.36	+41:56:43.10	1.63	AC0496-a							
J004112+412454	00:41:12.82	+41:24:54.38	9.01	AH0524-a							
J004114+412454	00:41:14.03	+41:24:54.40	3.03	AB0679-b							
J004114+414339	00:41:14.21	+41:43:39.31	1.18	AC0496-a							
J004114+410923	00:41:14.82	+41:09:23.60	0.79	AH0524-a							
J004114+410632	00:41:14.99	+41:06:32.30	2.62	AB0437-a							
J004115+410633	00:41:15.12	+41:06:33.79	0.80	AH0524-a							
J004117+412316	00:41:17.91	+41:23:16.22	2.16	AB0551-a							
J004118+412311	00:41:18.23	+41:23:11.70	1.65	AH0524-a							
J004119+412314	00:41:19.17	+41:23:14.37	1.09	AB0679-b							
J004119+411039	00:41:19.85	+41:10:39.50	18.38	AB0491-a							
J004120+411042	00:41:20.00	+41:10:42.30	15.50	AC0101-a							
J004120+413945	00:41:20.08	+41:39:45.10	2.57	AB0647-a							
J004120+411048	00:41:20.24	+41:10:48.79	5.21	AH0139-a							
J004120+412550	00:41:20.37	+41:25:50.40	12.53	AC0308-1							
J004120+411045	00:41:20.93	+41:10:45.76	2.78	AT0149-a							
J004120+401230	00:41:20.95	+40:12:30.30	7.16	AM0464-a							
J004121+405321	00:41:21.02	+40:53:21.60	4.75	AC0308-1							
J004121+405306	00:41:21.75	+40:53:06.11	2.95	AH0524-a							
J004123+411339	00:41:23.39	+41:13:39.47	2.97	AT0149-a							
J004124+401233	00:41:24.11	+40:12:33.40	40.73	AC0308-3							
J004125+401244	00:41:25.37	+40:12:44.30	9.21	AM0464-a							
J004125+410605	00:41:25.55	+41:06:05.40	4.26	AB0437-b							
J004125+401240	00:41:25.77	+40:12:40.51	6.43	AH0221-a							
J004125+411209	00:41:25.84	+41:12:09.30	8.39	AB0437-a							
J004126+411203	00:41:26.28	+41:12:03.00	6.32	AC0308-1							
J004127+401511	00:41:27.38	+40:15:11.99	1.43	AM0464-a							
J004127+401501	00:41:27.70	+40:15:01.85	6.45	AH0221-a					24.19	1.07	-0.87
J004127+401508	00:41:27.75	+40:15:08.60	4.83	AC0308-3							
J004128+412312	00:41:28.26	+41:23:12.02	2.40	AT0149-a							
J004128+411227	00:41:28.81	+41:12:27.30	12.49	AB0491-a							
J004129+413536	00:41:29.23	+41:35:36.41	1.02	AC0496-a							
J004129+405059	00:41:29.76	+40:50:59.70	3.71	AB0491-a							
J004130+410501	00:41:30.61	+41:05:01.40	2.33	AB0491-a							
J004130+410507	00:41:30.69	+41:05:07.26	1.91	AB0551-a							
J004131+421007	00:41:31.86	+42:10:07.20	0.70	AC0496-a							
J004132+421036	00:41:32.13	+42:10:36.50	1.31	AC0496-a							
J004132+412429	00:41:32.19	+41:24:29.20	2.13	AB0647-a							
J004132+403336	00:41:32.98	+40:33:36.83	1.14	AM0464-a							
J004133+403338	00:41:33.29	+40:33:38.29	1.77	AB0491-a					8.60	0.55	-1.04
J004134+410102	00:41:34.14	+41:01:02.14	0.98	AB0491-a							
J004134+411450*	00:41:34.41	+41:14:50.00	2.21	AB0437-a							
J004135+410657*	00:41:35.63	+41:06:57.10	0.65	AH0524-a							
J004136+404838	00:41:36.82	+40:48:38.96	0.62	AM0464-a							
J004136+404844	00:41:36.92	+40:48:44.67	0.68	AB0491-a							
J004138+412613	00:41:38.86	+41:26:13.62	2.05	AT0149-a							
J004139+413034	00:41:39.14	+41:30:34.60	20.49	AC0308-3							
J004139+404942	00:41:39.20	+40:49:42.14	1.18	AM0464-a							
J004139+413028	00:41:39.23	+41:30:28.88	29.98	AH0524-a							
J004139+412125	00:41:39.30	+41:21:25.40	0.80	AH0524-a							
J004139+413033	00:41:39.31	+41:30:33.50	3.64	AM0464-a					76.31	8.81	-1.99
J004139+413038	00:41:39.57	+41:30:38.00	8.66	AB0647-b							
J004139+414252	00:41:39.59	+41:42:52.90	2.87	AB0647-a							
J004139+404937	00:41:39.63	+40:49:37.13	1.31	AB0491-a							
J004139+413040	00:41:39.64	+41:30:40.80	5.69	AB0647-a							
J004139+413035	00:41:39.65	+41:30:35.70	27.95	AC0101-a							
J004140+412126	00:41:40.11	+41:21:26.65	0.80	AB0679-b							
J004141+410343	00:41:41.34	+41:03:43.60	33.45	AH0139-a							
J004145+412618	00:41:45.05	+41:26:18.64	7.45	AH0524-a							
J004145+412626	00:41:45.24	+41:26:26.70	4.06	AC0308-3							
J004145+412623	00:41:45.36	+41:26:23.20	5.75	AB0551-a							
J004145+411633	00:41:45.70	+41:16:33.90	14.01	AC0308-1							
J004145+411640	00:41:45.88	+41:16:40.20	5.47	AB0437-a							
J004146+411638	00:41:46.06	+41:16:38.10	3.38	AH0524-a					3.87	0.50	-0.09
J004146+411635	00:41:46.19	+41:16:35.00	2.41	AM0464-a							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004146+411705	00:41:46.34	+41:17:05.50	4.03	AC0308-3							
J004146+411643	00:41:46.41	+41:16:43.30	5.01	AB0551-a							
J004146+411700	00:41:46.44	+41:17:00.30	0.99	AH0524-a							
J004147+411850	00:41:47.39	+41:18:50.35	21.32	AH0221-a							
J004147+411641	00:41:47.48	+41:16:41.00	3.35	AC0308-3							
J004147+411848	00:41:47.59	+41:18:48.90	21.36	AC0308-3					206.88	13.62	-1.49
J004151+411441	00:41:51.15	+41:14:41.80	6.23	AC0308-3							
J004151+411436	00:41:51.34	+41:14:36.97	8.00	AT0149-a							
J004151+405443	00:41:51.38	+40:54:43.60	2.51	AH0524-a							
J004151+412438	00:41:51.68	+41:24:38.85	4.38	AH0524-a							
J004151+405431	00:41:51.83	+40:54:31.70	2.39	AB0491-a							
J004151+420250	00:41:51.89	+42:02:50.10	0.78	AC0496-a							
J004152+412441	00:41:52.02	+41:24:41.50	4.35	AB0551-a							
J004152+404644	00:41:52.10	+40:46:44.60	3.91	AB0437-b							
J004152+404645	00:41:52.36	+40:46:45.90	3.58	AB0437-a							
J004152+402122	00:41:52.65	+40:21:22.10	5.78	AM0464-a							
J004153+402114	00:41:53.37	+40:21:14.80	8.94	AC0308-3							
J004153+402117	00:41:53.43	+40:21:17.30	9.62	AH0221-a					36.97	1.71	-0.88
J004153+414513	00:41:53.59	+41:45:13.80	3.16	AC0496-a							
J004155+413720	00:41:55.95	+41:37:20.10	1.93	AB0647-a							
J004157+413415	00:41:57.56	+41:34:15.55	2.66	AT0149-a							
J004200+415408	00:42:00.51	+41:54:08.39	0.76	AB0647-b							
J004200+415406	00:42:00.63	+41:54:06.00	2.47	AC0496-a							
J004202+415902	00:42:02.34	+41:59:02.30	3.24	AC0496-a							
J004202+402831	00:42:02.59	+40:28:31.30	6.53	AM0464-a							
J004202+412635	00:42:02.86	+41:26:35.39	4.83	AH0524-a							
J004202+402830	00:42:02.91	+40:28:30.40	12.73	AC0308-1							
J004202+402832	00:42:02.93	+40:28:32.40	11.31	AB0491-a							
J004202+402818	00:42:02.99	+40:28:18.20	6.64	AC0308-3							
J004203+402828	00:42:03.02	+40:28:28.22	13.96	AH0221-a					32.59	1.85	-0.56
J004203+405409	00:42:03.44	+40:54:09.10	5.15	AC0308-3							
J004203+402409	00:42:03.90	+40:24:09.40	2.45	AM0464-a							
J004204+412932	00:42:04.53	+41:29:32.30	2.41	AB0647-b							
J004204+404918	00:42:04.59	+40:49:18.50	2.86	AB0437-a							
J004204+402405	00:42:04.70	+40:24:05.52	9.91	AH0221-a					23.12	1.28	-0.56
J004205+402406	00:42:05.17	+40:24:06.70	6.31	AC0308-3							
J004205+405615	00:42:05.97	+40:56:15.70	1.49	AB0491-a							
J004206+402708	00:42:06.68	+40:27:08.90	2.12	AB0491-a							
J004209+412638	00:42:09.05	+41:26:38.21	0.93	AB0679-a							
J004209+412704	00:42:09.91	+41:27:04.02	1.15	AB0679-a							
J004210+410228	00:42:10.13	+41:02:28.70	1.24	AH0524-a							
J004211+421557	00:42:11.48	+42:15:57.30	0.43	AC0496-a							
J004211+421703	00:42:11.54	+42:17:03.80	9.43	AC0308-1							
J004211+421655	00:42:11.65	+42:16:55.90	33.17	AC0496-a							
J004212+414828	00:42:12.82	+41:48:28.00	4.40	AB0647-a							
J004213+421957	00:42:13.09	+42:19:57.40	7.14	AC0496-a							
J004213+405126	00:42:13.65	+40:51:26.80	3.94	AB0437-a							
J004214+405121	00:42:14.00	+40:51:21.70	4.11	AB0491-a							
J004214+413317	00:42:14.93	+41:33:17.55	3.54	AT0149-a							
J004215+412930	00:42:15.72	+41:29:30.50	8.58	AB0679-b							
J004216+400959	00:42:16.43	+40:09:59.70	14.36	AM0464-a							
J004217+400952	00:42:17.39	+40:09:52.60	76.02	AC0308-3							
J004217+400948	00:42:17.40	+40:09:48.70	534.10	AH0221-a					2184.89	104.78	-0.92
J004218+400959	00:42:18.00	+40:09:59.10	9.23	AC0308-1							
J004218+412921	00:42:18.44	+41:29:21.14	330.51	AH0524-a							
J004218+412925	00:42:18.50	+41:29:25.60	105.40	AC0308-3							
J004218+412922	00:42:18.63	+41:29:22.58	245.11	AH0139-a							
J004218+412927	00:42:18.69	+41:29:27.10	327.30	AH0221-a					1223.64	61.20	-0.86
J004218+412921	00:42:18.87	+41:29:21.67	268.20	AT0149-a							
J004218+412933	00:42:18.95	+41:29:33.10	275.90	AC0496-a							
J004219+412928	00:42:19.18	+41:29:28.10	120.60	AM0464-a							
J004219+405347	00:42:19.62	+40:53:47.00	2.49	AB0437-a							
J004219+405344	00:42:19.93	+40:53:44.19	1.14	AM0464-a							
J004220+412634	00:42:20.19	+41:26:34.43	4.00	AH0524-a							
J004220+405344	00:42:20.23	+40:53:44.30	2.66	AB0491-a							
J004220+412641	00:42:20.48	+41:26:41.30	5.00	AB0551-a							
J004221+410802	00:42:21.73	+41:08:02.30	5.19	AH0524-a							
J004221+410759	00:42:21.80	+41:07:59.70	3.50	AB0437-a							
J004221+410757	00:42:21.81	+41:07:57.30	3.80	AB0491-a							
J004222+401605	00:42:22.09	+40:16:05.39	12.79	AH0221-a					30.36	2.00	-0.57
J004222+405746	00:42:22.20	+40:57:46.40	2.26	AH0524-a							
J004222+405745	00:42:22.43	+40:57:45.30	2.24	AB0437-a							
J004222+405736	00:42:22.46	+40:57:36.10	0.63	AB0491-a							
J004222+405744	00:42:22.60	+40:57:44.60	1.45	AM0464-a							
J004222+414829	00:42:22.69	+41:48:29.50	1.04	AC0496-a							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004223+402955	00:42:23.07	+40:29:55.60	2.69	AC0308-3							
J004223+405249	00:42:23.09	+40:52:49.50	9.67	AC0308-3							
J004223+413615	00:42:23.66	+41:36:15.20	0.46	AC0496-a							
J004223+402836	00:42:23.74	+40:28:36.10	2.62	AB0491-a							
J004223+404413	00:42:23.81	+40:44:13.92	1.81	AB0491-a							
J004223+405517	00:42:23.84	+40:55:17.80	14.22	AC0308-3							
J004224+412310	00:42:24.33	+41:23:10.20	1.69	AM0464-a							
J004224+405325	00:42:24.61	+40:53:25.00	5.45	AC0308-3							
J004225+404619	00:42:25.11	+40:46:19.70	4.55	AC0308-3							
J004226+404522	00:42:26.06	+40:45:22.80	5.42	AC0308-3							
J004226+411802	00:42:26.23	+41:18:02.90	2.15	AH0524-a							
J004226+405312	00:42:26.39	+40:53:12.10	10.78	AC0308-1							
J004226+411227	00:42:26.71	+41:12:27.30	12.91	AC0308-3							
J004226+411807	00:42:26.80	+41:18:07.32	2.21	AB0551-a							
J004227+405536	00:42:27.36	+40:55:36.50	10.41	AC0308-1							
J004228+412751	00:42:28.16	+41:27:51.00	8.65	AC0308-1							
J004228+411033	00:42:28.30	+41:10:33.70	4.59	AC0308-3							
J004228+411755	00:42:28.98	+41:17:55.50	16.04	AC0308-1							
J004229+403821	00:42:29.93	+40:38:21.40	2.27	AB0491-a							
J004229+413313	00:42:29.99	+41:33:13.60	5.49	AC0496-a							
J004232+411144	00:42:32.54	+41:11:44.30	1.18	AH0524-a							
J004232+411405	00:42:32.69	+41:14:05.50	6.46	AC0308-1							
J004233+411052	00:42:33.22	+41:10:52.99	0.26	AB0679-a							
J004233+412929	00:42:33.41	+41:29:29.70	2.92	AB0647-b							
J004234+412116	00:42:34.62	+41:21:16.54	0.97	AB0551-a							
J004234+413649	00:42:34.68	+41:36:49.30	2.06	AC0496-a							
J004235+402233	00:42:35.86	+40:22:33.30	5.44	AC0308-1							
J004236+402228	00:42:36.11	+40:22:28.34	17.76	AH0221-a					50.16	2.68	-0.68
J004236+411923	00:42:36.28	+41:19:23.00	1.17	AM0464-a							
J004236+415736	00:42:36.32	+41:57:36.40	4.49	AM0464-a							
J004237+421712	00:42:37.64	+42:17:12.40	1.25	AC0496-a							
J004238+412503	00:42:38.03	+41:25:03.64	2.44	AT0149-a							
J004240+410233	00:42:40.36	+41:02:33.13	0.69	AB0491-a							
J004241+413106	00:42:41.58	+41:31:06.70	2.68	AM0464-a							
J004241+413127	00:42:41.69	+41:31:27.90	4.68	AC0308-1							
J004241+414709	00:42:41.78	+41:47:09.70	2.15	AB0647-b							
J004242+411947	00:42:42.20	+41:19:47.00	8.65	AC0308-1							
J004242+414721	00:42:42.99	+41:47:21.00	1.44	AC0496-a							
J004243+411531	00:42:43.48	+41:15:31.60	2.58	AH0524-a							
J004243+413508	00:42:43.61	+41:35:08.40	7.55	AC0101-a							
J004244+411624	00:42:44.70	+41:16:24.70	15.44	AM0464-a							
J004244+411617	00:42:44.75	+41:16:17.60	34.23	AH0524-a							
J004245+411557	00:42:45.20	+41:15:57.60	161.40	AC0308-1							
J004245+411608	00:42:45.46	+41:16:08.10	86.53	AB0491-a							
J004245+411538	00:42:45.66	+41:15:38.00	4.73	AM0464-a							
J004245+411620	00:42:45.73	+41:16:20.90	14.26	AB0679-a							
J004245+411608	00:42:45.75	+41:16:08.00	94.20	AB0551-a							
J004245+411602	00:42:45.91	+41:16:02.50	94.22	AC0101-a							
J004245+411621	00:42:45.91	+41:16:21.20	15.50	AB0679-b							
J004245+411552	00:42:45.93	+41:15:52.60	5.01	AM0464-a							
J004246+413649	00:42:46.04	+41:36:49.90	2.84	AB0679-b							
J004246+413356	00:42:46.69	+41:33:56.20	2.72	AB0679-a							
J004246+410124	00:42:46.93	+41:01:24.80	2.71	AH0524-a							
J004247+411354	00:42:47.03	+41:13:54.36	2.73	AC0101-a							
J004247+410122	00:42:47.04	+41:01:22.80	3.67	AB0437-a							
J004247+413346	00:42:47.08	+41:33:46.90	3.52	AB0647-a							
J004247+413338	00:42:47.14	+41:33:38.60	6.24	AB0551-a							
J004247+413341	00:42:47.34	+41:33:41.50	9.48	AB0647-b							
J004247+411519	00:42:47.68	+41:15:19.90	2.59	AM0464-a							
J004248+404558	00:42:48.41	+40:45:58.06	0.77	AB0491-a							
J004248+413352	00:42:48.52	+41:33:52.50	6.89	AC0308-1							
J004248+411939	00:42:48.62	+41:19:39.73	1.90	AB0551-a							
J004248+412408	00:42:48.71	+41:24:08.39	1.02	AB0551-a							
J004248+411606	00:42:48.98	+41:16:06.80	20.10	AC0308-2							
J004249+411604	00:42:49.85	+41:16:04.20	8.07	AH0524-a							
J004250+413905	00:42:50.32	+41:39:05.70	2.79	AB0679-b							
J004250+411601	00:42:50.36	+41:16:01.80	4.28	AM0464-a							
J004250+413855	00:42:50.93	+41:38:55.90	2.68	AB0679-b							
J004250+421141	00:42:50.96	+42:11:41.50	2.90	AC0496-a							
J004251+413317	00:42:51.03	+41:33:17.80	1.19	AM0464-a							
J004251+412628	00:42:51.13	+41:26:28.66	19.73	AH0524-a							
J004251+412631	00:42:51.37	+41:26:31.90	19.68	AH0139-a							
J004251+412627	00:42:51.51	+41:26:27.77	9.17	AT0149-a							
J004251+412635	00:42:51.88	+41:26:35.60	18.33	AM0464-a							
J004252+413557	00:42:52.22	+41:35:57.10	4.73	AC0308-1							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004252+413745	00:42:52.51	+41:37:45.60	1.90	AB0679-a							
J004253+414854	00:42:53.32	+41:48:54.30	0.62	AC0496-a							
J004254+413826	00:42:54.30	+41:38:26.00	3.96	AB0679-b							
J004254+413822	00:42:54.44	+41:38:22.80	2.76	AB0679-a							
J004254+422120	00:42:54.98	+42:21:20.08	2.21	AC0496-a							
J004255+413708	00:42:55.67	+41:37:08.40	2.02	AB0679-a							
J004256+414748	00:42:56.26	+41:47:48.00	1.23	AC0496-a							
J004257+411643	00:42:57.84	+41:16:43.80	8.25	AC0308-2							
J004257+413742	00:42:57.91	+41:37:42.70	6.26	AB0679-a							
J004259+413654	00:42:59.46	+41:36:54.90	14.41	AC0308-1							
J004300+413348	00:43:00.56	+41:33:48.50	4.16	AC0308-1							
J004301+413735	00:43:01.97	+41:37:35.00	4.67	AB0647-b							
J004303+413832	00:43:03.35	+41:38:32.20	3.09	AB0679-b							
J004303+413723	00:43:03.39	+41:37:23.50	5.79	AB0647-a							
J004304+413846	00:43:04.44	+41:38:46.80	3.95	AB0647-b							
J004304+413758	00:43:04.48	+41:37:58.00	17.31	AC0308-1							
J004305+413755	00:43:05.89	+41:37:55.25	0.96	AC0496-a							
J004306+413420	00:43:06.25	+41:34:20.90	3.12	AB0647-a							
J004306+413340	00:43:06.63	+41:33:40.10	3.33	AC0308-1							
J004306+413810	00:43:06.69	+41:38:10.20	2.55	AB0679-b							
J004306+413618	00:43:06.75	+41:36:18.50	8.02	AC0101-a							
J004307+415511	00:43:07.13	+41:55:11.90	4.80	AC0308-1							
J004308+415501	00:43:08.06	+41:55:01.10	2.06	AB0647-b							
J004308+415506	00:43:08.19	+41:55:06.50	2.38	AC0496-a							
J004308+402846	00:43:08.96	+40:28:46.60	5.49	AC0308-1							
J004309+402844	00:43:09.58	+40:28:44.91	7.23	AH0221-a					75.41	3.68	-1.54
J004309+402847	00:43:09.60	+40:28:47.70	17.32	AB0491-a							
J004314+413806	00:43:14.85	+41:38:06.30	5.59	AC0308-1							
J004317+411720	00:43:17.43	+41:17:20.95	4.09	AH0524-a							
J004317+411722	00:43:17.77	+41:17:22.76	4.02	AH0139-a							
J004318+411730	00:43:18.24	+41:17:30.80	5.83	AC0308-1							
J004318+412425	00:43:18.61	+41:24:25.32	0.98	AB0551-a							
J004318+411727	00:43:18.62	+41:17:27.30	2.76	AB0647-b							
J004319+405633	00:43:19.67	+40:56:33.00	5.53	AC0101-a							
J004324+413459	00:43:24.29	+41:34:59.90	6.34	AC0308-1							
J004325+412235	00:43:25.33	+41:22:35.90	5.02	AC0308-1							
J004326+411913	00:43:26.44	+41:19:13.10	4.68	AM0464-a							
J004326+420723	00:43:26.48	+42:07:23.60	1.18	AC0496-a							
J004326+411915	00:43:26.87	+41:19:15.80	1.99	AB0647-b							
J004327+413512	00:43:27.52	+41:35:12.10	2.48	AB0679-a							
J004327+413514	00:43:27.66	+41:35:14.20	3.58	AM0464-a							
J004327+413528	00:43:27.72	+41:35:28.60	3.38	AB0647-a							
J004327+413523	00:43:27.74	+41:35:23.60	3.20	AB0679-b							
J004328+413511	00:43:28.24	+41:35:11.00	17.19	AC0308-1							
J004328+420644	00:43:28.71	+42:06:44.80	0.58	AC0496-a							
J004329+413547	00:43:29.18	+41:35:47.70	21.03	AB0647-b							
J004330+413557	00:43:30.07	+41:35:57.50	2.04	AM0464-a							
J004330+413353	00:43:30.47	+41:33:53.03	2.22	AT0149-a							
J004332+413623	00:43:32.82	+41:36:23.70	3.35	AM0464-a							
J004333+413941	00:43:33.30	+41:39:41.00	5.44	AC0308-1							
J004333+415955	00:43:33.38	+41:59:55.30	0.98	AC0496-a							
J004334+413605	00:43:34.46	+41:36:05.48	2.18	AT0149-a							
J004334+421200	00:43:34.73	+42:12:00.80	3.03	AC0308-1							
J004334+410951	00:43:34.78	+41:09:51.90	7.72	AM0464-a							
J004335+421219	00:43:35.23	+42:12:19.90	3.64	AC0308-2							
J004335+414444	00:43:35.80	+41:44:44.70	0.47	AC0496-a							
J004336+403809	00:43:36.72	+40:38:09.30	4.41	AB0491-a							
J004336+412026	00:43:36.95	+41:20:26.20	9.80	AB0647-b							
J004337+412019	00:43:37.28	+41:20:19.40	8.92	AC0308-2							
J004337+414007	00:43:37.80	+41:40:07.30	3.14	AB0647-a							
J004338+414008	00:43:38.57	+41:40:08.10	5.80	AB0647-b					14.97	0.93	-0.62
J004338+414005	00:43:38.77	+41:40:05.93	4.50	AM0464-a							
J004338+412652	00:43:38.87	+41:26:52.56	2.65	AB0551-a							
J004339+413959	00:43:39.14	+41:39:59.30	5.24	AC0308-1							
J004340+414318	00:43:40.84	+41:43:18.90	2.99	AC0496-a							
J004340+405428	00:43:40.92	+40:54:28.20	58.80	AB0491-a							
J004340+405431	00:43:40.92	+40:54:31.60	35.75	AM0464-a							
J004341+405434	00:43:41.17	+40:54:34.00	52.80	AB0551-a							
J004341+405435	00:43:41.76	+40:54:35.90	9.40	AC0308-2							
J004342+414533	00:43:42.50	+41:45:33.38	0.46	AB0647-b							
J004343+411232	00:43:43.67	+41:12:32.41	0.35	AB0679-a							
J004343+412839	00:43:43.94	+41:28:39.98	17.33	AH0139-a							
J004344+412841	00:43:44.22	+41:28:41.20	24.99	AC0308-1							
J004344+412845	00:43:44.89	+41:28:45.60	22.53	AC0101-a							
J004345+411219	00:43:45.22	+41:12:19.70	7.94	AC0101-a							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004345+412839	00:43:45.22	+41:28:39.90	4.91	AC0308-2							
J004346+414252	00:43:46.86	+41:42:52.40	0.44	AC0496-a							
J004351+414256	00:43:51.56	+41:42:56.56	0.51	AB0647-b							
J004351+403923	00:43:51.89	+40:39:23.60	3.24	AB0491-a							
J004351+414424	00:43:51.99	+41:44:24.08	0.79	AB0647-b							
J004352+412854	00:43:52.86	+41:28:54.66	0.78	AM0464-a							
J004354+404640	00:43:54.00	+40:46:40.70	35.69	AM0464-a							
J004354+404635	00:43:54.08	+40:46:35.40	134.80	AB0491-a							
J004354+411210	00:43:54.51	+41:12:10.00	0.79	AB0551-a							
J004355+404648	00:43:55.44	+40:46:48.70	6.45	AC0308-2							
J004356+412626	00:43:56.24	+41:26:26.62	1.35	AB0551-a							
J004356+413906	00:43:56.92	+41:39:06.25	1.33	AC0496-a							
J004357+415717	00:43:57.43	+41:57:17.76	1.67	AH0221-a							
J004357+415716	00:43:57.83	+41:57:16.70	2.42	AH0221-a							
J004358+411332	00:43:58.18	+41:13:32.96	0.69	AB0551-a							
J004358+421523	00:43:58.93	+42:15:23.50	5.42	AC0308-2							
J004358+421518	00:43:58.94	+42:15:18.10	5.66	AC0308-1							
J004359+415713	00:43:59.34	+41:57:13.60	34.64	AM0464-a							
J004359+415722	00:43:59.34	+41:57:22.60	23.25	AC0308-2							
J004401+414908	00:44:01.38	+41:49:08.20	4.11	AB0647-a							
J004401+414907	00:44:01.61	+41:49:07.60	3.64	AM0464-a							
J004401+414911	00:44:01.68	+41:49:11.20	5.59	AB0647-b							
J004402+411222	00:44:02.56	+41:12:22.69	0.70	AB0551-a							
J004402+414426	00:44:02.58	+41:44:26.73	0.92	AB0647-b							
J004402+414917	00:44:02.63	+41:49:17.50	5.33	AC0308-1							
J004403+411854	00:44:03.34	+41:18:54.10	6.97	AC0308-1							
J004403+411715	00:44:03.46	+41:17:15.26	1.57	AB0551-a							
J004405+410734	00:44:05.06	+41:07:34.27	1.36	AB0551-a							
J004405+414939	00:44:05.82	+41:49:39.90	1.09	AC0496-a							
J004405+411112	00:44:05.87	+41:11:12.21	1.35	AB0551-a							
J004406+411849	00:44:06.26	+41:18:49.24	1.33	AB0551-a							
J004407+413111	00:44:07.41	+41:31:11.50	8.11	AM0464-a							
J004407+413107	00:44:07.72	+41:31:07.90	8.67	AB0551-a							
J004407+421111	00:44:07.82	+42:11:11.50	0.22	AC0496-a							
J004407+413107	00:44:07.92	+41:31:07.30	6.45	AC0308-1							
J004407+413110	00:44:07.92	+41:31:10.20	6.37	AB0647-b							
J004408+413108	00:44:08.13	+41:31:08.00	4.92	AB0647-a							
J004409+413321	00:44:09.56	+41:33:21.50	1.53	AM0464-a							
J004410+413319	00:44:10.05	+41:33:19.21	1.95	AB0647-b							
J004410+422548	00:44:10.71	+42:25:48.70	14.73	AC0308-2							
J004410+420108	00:44:10.99	+42:01:08.60	1.19	AC0496-a							
J004413+411953	00:44:13.12	+41:19:53.64	0.72	AB0679-b							
J004413+412759	00:44:13.28	+41:27:59.20	7.16	AC0101-a							
J004413+411954*	00:44:13.52	+41:19:54.70	1.89	AM0464-a							
J004414+411946	00:44:14.01	+41:19:46.60	0.80	AB0647-a							
J004414+411953	00:44:14.16	+41:19:53.69	1.11	AB0647-b							
J004415+413057	00:44:15.93	+41:30:57.90	1.40	AM0464-a							
J004417+411340	00:44:17.13	+41:13:40.92	5.66	AH0139-a							
J004417+411345	00:44:17.96	+41:13:45.20	12.85	AC0101-a							
J004418+411338	00:44:18.37	+41:13:38.08	10.01	AH0221-a					36.57	1.62	-0.85
J004418+411342	00:44:18.53	+41:13:42.80	5.85	AB0647-b							
J004419+415152	00:44:19.04	+41:51:52.40	0.58	AB0647-b							
J004419+411337	00:44:19.04	+41:13:37.90	4.60	AC0308-1							
J004420+411755	00:44:20.80	+41:17:55.27	0.69	AB0551-a							
J004420+411747	00:44:20.91	+41:17:47.81	1.39	AB0647-b							
J004423+413034	00:44:23.10	+41:30:34.60	19.49	AB0679-b							
J004423+413035	00:44:23.35	+41:30:35.50	13.66	AB0679-a							
J004423+413041	00:44:23.52	+41:30:41.50	10.19	AC0308-1							
J004423+412054	00:44:23.81	+41:20:54.48	1.40	AB0647-a							
J004424+413041	00:44:24.07	+41:30:41.80	12.98	AM0464-a							
J004424+413036	00:44:24.08	+41:30:36.00	4.45	AC0308-2							
J004424+413041	00:44:24.33	+41:30:41.66	2.62	AH0221-a					25.98	1.12	-1.50
J004424+415422	00:44:24.42	+41:54:22.60	1.72	AC0496-a							
J004424+414922	00:44:24.64	+41:49:22.71	1.05	AB0647-b							
J004424+412103	00:44:24.66	+41:21:03.80	13.84	AC0308-2							
J004424+415424	00:44:24.78	+41:54:24.50	8.29	AC0308-1							
J004424+412058	00:44:24.81	+41:20:58.10	4.38	AB0647-b							
J004424+415419	00:44:24.95	+41:54:19.70	3.56	AM0464-a							
J004425+411530	00:44:25.09	+41:15:30.10	6.06	AC0101-a							
J004425+411528	00:44:25.96	+41:15:28.10	2.68	AH0221-a							
J004426+411525	00:44:26.15	+41:15:25.00	8.18	AB0551-a							
J004426+411526	00:44:26.85	+41:15:26.80	9.93	AC0308-2							
J004426+411520	00:44:26.94	+41:15:20.25	2.52	AH0221-a							
J004427+411526	00:44:27.11	+41:15:26.80	4.39	AC0308-1							
J004429+411126	00:44:29.22	+41:11:26.80	19.64	AC0101-a							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004430+415158	00:44:30.61	+41:51:58.00	3.61	AB0647-b							
J004430+415241	00:44:30.87	+41:52:41.90	20.45	AC0308-1							
J004432+412352	00:44:32.57	+41:23:52.39	1.12	AB0647-a							
J004434+414508	00:44:34.44	+41:45:08.10	29.61	AM0464-a							
J004435+412534	00:44:35.47	+41:25:34.00	15.54	AC0308-1							
J004435+412518	00:44:35.65	+41:25:18.90	3.58	AM0464-a							
J004436+412520	00:44:36.76	+41:25:20.90	10.76	AC0308-2							
J004437+412518	00:44:37.15	+41:25:18.70	8.05	AB0647-a							
J004437+414517	00:44:37.23	+41:45:17.00	5.85	AC0308-2							
J004437+412516	00:44:37.32	+41:25:16.80	10.69	AB0647-b							
J004437+412506	00:44:37.59	+41:25:06.60	1.91	AB0679-a							
J004437+414521	00:44:37.65	+41:45:21.10	6.23	AC0308-1							
J004437+412519	00:44:37.68	+41:25:19.60	13.97	AB0551-a							
J004438+420404	00:44:38.21	+42:04:04.80	4.75	AC0308-2							
J004438+412513	00:44:38.35	+41:25:13.00	2.70	AM0464-a							
J004438+422216	00:44:38.36	+42:22:16.40	11.87	AC0308-2							
J004439+424752	00:44:39.67	+42:47:52.60	8.96	AC0308-2							
J004441+420402	00:44:41.71	+42:04:02.70	0.96	AB0647-b							
J004443+412733	00:44:43.29	+41:27:33.20	7.54	AC0308-1							
J004444+412658	00:44:44.12	+41:26:58.40	8.67	AC0308-2							
J004444+412745	00:44:44.15	+41:27:45.80	4.73	AB0647-b							
J004444+412748	00:44:44.18	+41:27:48.97	1.14	AB0647-a							
J004444+412640	00:44:44.58	+41:26:40.60	7.62	AC0308-1							
J004445+415152	00:44:45.08	+41:51:52.63	1.28	AB0647-b							
J004446+415743	00:44:46.71	+41:57:43.57	1.07	AB0647-b							
J004447+420816	00:44:47.86	+42:08:16.85	1.51	AB0647-b							
J004447+420819	00:44:47.92	+42:08:19.80	2.96	AC0308-2					8.48	0.65	-0.69
J004450+415957	00:44:50.43	+41:59:57.59	1.58	AB0647-a							
J004450+415952	00:44:50.89	+41:59:52.20	2.66	AB0647-b							
J004452+415455	00:44:52.24	+41:54:55.82	0.87	AB0647-a							
J004452+415456*	00:44:52.61	+41:54:56.22	1.50	AB0647-b							
J004452+415454	00:44:52.98	+41:54:54.87	0.62	AM0464-a							
J004453+414049	00:44:53.16	+41:40:49.30	25.18	AM0464-a							
J004455+414324	00:44:55.99	+41:43:24.40	3.10	AC0308-2							
J004458+413139	00:44:58.68	+41:31:39.80	5.54	AB0647-b							
J004458+414254	00:44:58.80	+41:42:54.10	3.06	AC0308-1							
J004500+412837	00:45:00.03	+41:28:37.44	1.51	AB0647-b							
J004500+420352	00:45:00.17	+42:03:52.49	1.03	AB0647-b							
J004500+412835	00:45:00.72	+41:28:35.52	0.93	AB0647-a							
J004501+412458	00:45:01.56	+41:24:58.20	20.79	AC0308-1							
J004501+412455	00:45:01.74	+41:24:55.75	9.80	AH0221-a							
J004501+412206	00:45:01.90	+41:22:06.60	10.33	AM0464-a							
J004502+412451	00:45:02.08	+41:24:51.80	37.96	AC0308-2							
J004502+414138	00:45:02.85	+41:41:38.70	0.91	AM0464-a							
J004503+405341	00:45:03.74	+40:53:41.19	10.60	AH0221-a							
J004503+413952	00:45:03.94	+41:39:52.68	1.50	AB0647-b							
J004503+405342	00:45:03.95	+40:53:42.20	25.40	AC0308-1							
J004504+405347	00:45:04.25	+40:53:47.14	2.91	AM0464-a							
J004504+405347	00:45:04.47	+40:53:47.90	17.29	AC0308-2							
J004504+405347	00:45:04.70	+40:53:47.03	15.55	AH0221-a							
J004505+412233	00:45:05.14	+41:22:33.50	25.37	AC0308-2							
J004505+412238	00:45:05.19	+41:22:38.10	17.22	AB0647-a							
J004505+412244	00:45:05.24	+41:22:44.40	5.47	AC0308-1							
J004505+412240	00:45:05.41	+41:22:40.90	21.72	AB0647-b							
J004505+405135	00:45:05.63	+40:51:35.90	5.50	AC0308-1							
J004505+412244	00:45:05.73	+41:22:44.40	19.28	AM0464-a					58.47	6.90	-0.73
J004506+413423	00:45:06.08	+41:34:23.95	0.93	AM0464-a							
J004506+405128	00:45:06.41	+40:51:28.30	3.03	AC0308-2							
J004509+414942	00:45:09.17	+41:49:42.42	0.69	AM0464-a							
J004509+415003	00:45:09.68	+41:50:03.80	2.08	AM0464-a							
J004510+410927	00:45:10.36	+41:09:27.00	17.69	AM0464-a							
J004510+413255	00:45:10.88	+41:32:55.25	2.05	AB0647-b							
J004511+411124	00:45:11.18	+41:11:24.70	9.65	AC0308-1							
J004511+411152	00:45:11.42	+41:11:52.70	103.60	AC0308-2							
J004511+410854	00:45:11.70	+41:08:54.05	5.79	AH0221-a					24.97	1.37	-0.96
J004511+411131	00:45:11.79	+41:11:31.44	19.95	AH0221-a							
J004512+413712	00:45:12.35	+41:37:12.30	2.60	AM0464-a							
J004512+413714	00:45:12.35	+41:37:14.50	5.03	AB0647-b							
J004512+413659	00:45:12.52	+41:36:59.46	1.41	AB0647-a							
J004512+412053	00:45:12.71	+41:20:53.23	0.43	AM0464-a							
J004513+413610	00:45:13.77	+41:36:10.40	3.55	AB0647-b							
J004513+413701	00:45:13.88	+41:37:01.70	8.08	AC0308-2							
J004513+413616*	00:45:13.98	+41:36:16.60	2.60	AM0464-a							
J004516+411907	00:45:16.83	+41:19:07.70	4.50	AC0308-2							
J004517+405700	00:45:17.32	+40:57:00.37	14.91	AH0221-a					8.52	0.58	0.37

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004517+405705	00:45:17.79	+40:57:05.30	3.16	AC0308-2							
J004517+410647	00:45:17.96	+41:06:47.31	3.58	AH0221-a					4.25	0.49	-0.11
J004520+413933	00:45:20.00	+41:39:33.88	1.63	AB0647-b							
J004520+413934	00:45:20.85	+41:39:34.60	1.78	AM0464-a							
J004521+403744	00:45:21.36	+40:37:44.20	4.58	AC0308-1							
J004524+415541	00:45:24.04	+41:55:41.55	2.12	AB0647-b							
J004524+415535	00:45:24.41	+41:55:35.80	1.31	AM0464-a					4.98	0.62	-0.88
J004525+414553	00:45:25.88	+41:45:53.80	4.57	AC0308-2							
J004527+414309	00:45:27.00	+41:43:09.13	0.82	AB0647-a							
J004527+414259	00:45:27.06	+41:42:59.83	1.46	AB0647-b							
J004527+414303*	00:45:27.64	+41:43:03.20	2.05	AM0464-a							
J004529+414456	00:45:29.50	+41:44:56.47	1.45	AB0647-b							
J004537+414658	00:45:37.33	+41:46:58.70	6.00	AC0308-2							
J004537+405200	00:45:37.77	+40:52:00.38	4.78	AH0221-a					15.35	1.04	-0.76
J004538+404627	00:45:38.10	+40:46:27.00	8.70	AC0308-1							
J004538+414715	00:45:38.98	+41:47:15.58	1.21	AB0647-a							
J004539+414712*	00:45:39.53	+41:47:12.20	1.15	AM0464-a							
J004539+411221	00:45:39.67	+41:12:21.30	17.04	AM0464-a							
J004539+411225	00:45:39.76	+41:12:25.68	12.85	AH0221-a							
J004539+411223	00:45:39.87	+41:12:23.20	8.39	AB0647-a							
J004539+411220	00:45:39.95	+41:12:20.00	12.72	AB0647-b					109.30	8.91	-1.41
J004540+411214	00:45:40.11	+41:12:14.00	39.35	AC0308-2							
J004542+412106	00:45:42.48	+41:21:06.90	3.36	AC0308-2							
J004542+411123	00:45:42.49	+41:11:23.40	4.12	AM0464-a							
J004542+415518	00:45:42.74	+41:55:18.30	8.38	AC0308-2							
J004542+415303	00:45:42.80	+41:53:03.72	1.14	AB0647-b							
J004543+411118	00:45:43.03	+41:11:18.30	9.73	AH0221-a					35.01	1.69	-0.84
J004543+415259	00:45:43.05	+41:52:59.51	0.85	AM0464-a							
J004544+404425	00:45:44.01	+40:44:25.69	1.75	AH0221-a					46.56	2.57	-2.15
J004553+413314	00:45:53.32	+41:33:14.04	1.09	AB0647-a							
J004553+413320	00:45:53.52	+41:33:20.21	0.65	AM0464-a							
J004554+413318	00:45:54.06	+41:33:18.07	2.42	AB0647-b							
J004555+415642	00:45:55.13	+41:56:42.74	0.91	AM0464-a							
J004556+415614	00:45:56.47	+41:56:14.86	2.03	AB0647-b							
J004557+415610	00:45:57.29	+41:56:10.32	0.51	AB0647-a							
J004557+415607	00:45:57.61	+41:56:07.94	2.69	AH0221-a					7.00	0.55	-0.63
J004557+415605	00:45:57.63	+41:56:05.80	1.78	AM0464-a							
J004601+412321	00:46:01.61	+41:23:21.40	2.19	AB0647-b							
J004601+412318	00:46:01.64	+41:23:18.65	1.11	AM0464-a							
J004601+412319	00:46:01.81	+41:23:19.96	0.90	AB0647-a							
J004602+412322	00:46:02.34	+41:23:22.60	4.77	AC0308-2							
J004602+404806	00:46:02.56	+40:48:06.35	30.82	AH0221-a					327.84	16.52	-1.55
J004602+404811	00:46:02.96	+40:48:11.90	7.48	AC0308-2							
J004605+422035	00:46:05.85	+42:20:35.23	4.47	AH0221-a					12.09	0.86	-0.65
J004606+422044	00:46:06.21	+42:20:44.30	5.86	AC0308-2							
J004608+420349	00:46:08.75	+42:03:49.21	0.67	AM0464-a							
J004608+420522	00:46:08.89	+42:05:22.50	2.44	AC0308-2							
J004608+420357	00:46:08.93	+42:03:57.13	3.29	AH0221-a							
J004609+415449	00:46:09.09	+41:54:49.50	4.75	AC0308-2							
J004609+415439	00:46:09.19	+41:54:39.90	2.99	AB0647-b							
J004609+420525	00:46:09.23	+42:05:25.01	3.48	AH0221-a					8.27	0.67	-0.57
J004609+421900	00:46:09.42	+42:19:00.90	4.99	AC0308-2							
J004609+415438	00:46:09.50	+41:54:38.40	3.68	AM0464-a							
J004609+415301	00:46:09.61	+41:53:01.50	3.58	AC0308-2							
J004609+412315	00:46:09.62	+41:23:15.44	0.96	AM0464-a							
J004609+422203	00:46:09.66	+42:22:03.54	3.59	AH0221-a					13.72	1.03	-0.88
J004609+412312	00:46:09.73	+41:23:12.61	1.45	AB0647-a							
J004610+422158	00:46:10.14	+42:21:58.40	4.73	AC0308-2							
J004610+412314	00:46:10.60	+41:23:14.68	1.76	AB0647-b							
J004610+412316	00:46:10.87	+41:23:16.70	3.41	AC0308-2							
J004611+420412	00:46:11.41	+42:04:12.71	1.72	AB0647-a							
J004612+420405	00:46:12.40	+42:04:05.00	2.25	AM0464-a							
J004612+404708	00:46:12.48	+40:47:08.98	5.41	AH0221-a							
J004612+420413	00:46:12.79	+42:04:13.47	5.99	AH0221-a					14.37	0.84	-0.57
J004615+404652	00:46:15.45	+40:46:52.33	4.64	AH0221-a							
J004617+414232	00:46:17.21	+41:42:32.10	1.32	AM0464-a							
J004620+412447	00:46:20.88	+41:24:47.45	1.45	AB0647-b							
J004621+412446	00:46:21.17	+41:24:46.60	4.48	AC0308-2					7.14	0.53	-0.31
J004621+414422	00:46:21.95	+41:44:22.50	2.73	AB0647-b							
J004622+414420	00:46:22.16	+41:44:20.00	6.02	AM0464-a							
J004622+414423	00:46:22.22	+41:44:23.49	1.37	AB0647-a							
J004622+414419	00:46:22.66	+41:44:19.50	3.27	AC0308-2							
J004626+411935	00:46:26.32	+41:19:35.80	11.06	AM0464-a							
J004626+411933	00:46:26.94	+41:19:33.84	4.05	AH0221-a					168.69	11.57	-2.44
J004627+411936	00:46:27.09	+41:19:36.20	49.17	AC0308-2							

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
J004629+413759	00:46:29.65	+41:37:59.90	4.71	AC0308-2							
J004632+422349	00:46:32.07	+42:23:49.28	2.56	AH0221-a					7.84	0.90	-0.73
J004633+421141	00:46:33.94	+42:11:41.00	6.77	AC0308-2							
J004634+422653	00:46:34.60	+42:26:53.80	9.87	AC0308-2							
J004635+422651	00:46:35.06	+42:26:51.46	8.04	AH0221-a							
J004635+422714	00:46:35.28	+42:27:14.09	5.49	AH0221-a							
J004636+423154	00:46:36.79	+42:31:54.80	7.80	AC0308-2							
J004636+423158	00:46:36.96	+42:31:58.40	33.96	AH0221-a					146.43	7.22	-0.96
J004637+415342	00:46:37.00	+41:53:42.20	0.98	AM0464-a							
J004637+405425	00:46:37.32	+40:54:25.90	9.13	AC0308-2							
J004638+405423	00:46:38.60	+40:54:23.52	8.01	AH0221-a							
J004639+421235	00:46:39.44	+42:12:35.55	8.38	AH0221-a					13.60	1.01	-0.32
J004640+415419	00:46:40.17	+41:54:19.90	1.47	AM0464-a							
J004640+421235	00:46:40.19	+42:12:35.20	9.90	AC0308-2							
J004640+415423	00:46:40.62	+41:54:23.41	2.48	AH0221-a							
J004641+414040	00:46:41.57	+41:40:40.84	1.07	AB0647-b							
J004641+414036	00:46:41.64	+41:40:36.40	3.09	AM0464-a							
J004641+415450	00:46:41.72	+41:54:50.35	1.72	AB0647-b							
J004641+414036	00:46:41.85	+41:40:36.80	8.53	AC0308-2							
J004642+415500	00:46:42.38	+41:55:00.00	2.94	AM0464-a							
J004642+415503	00:46:42.73	+41:55:03.17	2.12	AH0221-a					12.22	0.78	-1.15
J004643+415502	00:46:43.29	+41:55:02.70	9.10	AC0308-2							
J004645+412901	00:46:45.26	+41:29:01.54	0.33	AM0464-a							
J004646+414314	00:46:46.19	+41:43:14.00	3.06	AC0308-2							
J004647+411406	00:46:47.23	+41:14:06.27	0.35	AM0464-a							
J004647+420848	00:46:47.79	+42:08:48.60	18.02	AM0464-a							
J004647+421410	00:46:47.98	+42:14:10.60	10.43	AC0308-2							
J004648+420854	00:46:48.11	+42:08:54.40	123.20	AC0308-2							
J004648+420856	00:46:48.19	+42:08:56.90	111.50	AH0221-a					450.86	19.58	-0.92
J004648+411417	00:46:48.23	+41:14:17.60	16.28	AC0308-2							
J004648+411404	00:46:48.84	+41:14:04.66	1.28	AB0647-b							
J004649+411403	00:46:49.04	+41:14:03.69	8.63	AH0221-a					52.49	2.82	-1.18
J004650+410451	00:46:50.98	+41:04:51.70	1.97	AC0308-2							
J004651+421602	00:46:51.58	+42:16:02.90	2.54	AC0308-2							
J004651+410446	00:46:51.77	+41:04:46.76	6.30	AH0221-a					34.51	1.95	-1.11
J004653+414908	00:46:53.36	+41:49:08.64	1.70	AB0647-a							
J004653+414911	00:46:53.44	+41:49:11.30	10.24	AC0308-2							
J004657+411141	00:46:57.66	+41:11:41.00	3.63	AC0308-2							
J004702+413139	00:47:02.61	+41:31:39.40	4.20	AC0308-2							
J004709+414246	00:47:09.38	+41:42:46.00	1.35	AM0464-a							
J004713+414023	00:47:13.85	+41:40:23.44	1.37	AM0464-a							
J004714+414022	00:47:14.37	+41:40:22.12	4.17	AH0221-a							
J004722+415851	00:47:22.56	+41:58:51.01	0.94	AM0464-a							
J004723+415855	00:47:23.32	+41:58:55.90	5.08	AC0308-2					13.73	0.75	-0.65
J004725+413205	00:47:25.85	+41:32:05.84	1.31	AM0464-a							
J004726+413202	00:47:26.56	+41:32:02.30	12.67	AC0308-2							
J004726+421910	00:47:26.98	+42:19:10.10	2.67	AC0308-2							
J004726+413158	00:47:26.99	+41:31:58.76	9.71	AH0221-a					49.06	2.00	-1.06
J004730+414921	00:47:30.31	+41:49:21.17	1.46	AM0464-a							
J004730+414921	00:47:30.77	+41:49:21.40	2.89	AC0308-2							
J004731+414925	00:47:31.27	+41:49:25.54	3.00	AH0221-a					13.75	0.71	-1.00
J004736+420337	00:47:36.75	+42:03:37.30	2.11	AC0308-2							
J004738+422023	00:47:38.54	+42:20:23.56	8.30	AH0221-a							
J004748+414152	00:47:48.66	+41:41:52.99	0.74	AM0464-a							
J004749+414152	00:47:49.10	+41:41:52.71	4.57	AH0221-a							
J004749+414148	00:47:49.61	+41:41:48.60	7.10	AC0308-2							
J004749+414147	00:47:49.99	+41:41:47.79	5.91	AH0221-a							
J004756+413234	00:47:56.82	+41:32:34.61	2.47	AH0221-a							
J004808+423656	00:48:08.39	+42:36:56.56	2.51	AH0221-a							
J004822+422502	00:48:22.92	+42:25:02.70	3.24	AC0308-2							
J004830+413718	00:48:30.76	+41:37:18.32	4.67	AH0221-a					19.35	1.23	-0.93
J004845+413658	00:48:45.46	+41:36:58.90	4.19	AC0308-2							
J004846+413706	00:48:46.92	+41:37:06.97	2.06	AH0221-a							
J004903+420801	00:49:03.76	+42:08:01.62	1.44	AH0221-a							
J004911+413557	00:49:11.50	+41:35:57.53	2.14	AH0221-a					13.02	0.85	-1.18
J004912+415702	00:49:12.99	+41:57:02.33	2.89	AH0221-a					71.33	3.38	-2.10
J004939+413718	00:49:39.56	+41:37:18.68	2.21	AH0221-a							
J003949+410420	00:39:49.61	+41:04:20.70	10.51	AB0437-a	1	3	7.87	33.49			
	00:39:49.70	+41:04:21.20	6.40	AM0464-a	1	3					
	00:39:49.75	+41:04:19.80	6.71	AC0308-3	1	3					
J003956+411137	00:39:56.54	+41:11:37.00	75.94	AB0437-a	2	3	57.24	32.67			
	00:39:56.57	+41:11:37.90	49.49	AC0308-3	2	3					
	00:39:56.62	+41:11:36.80	46.29	AM0464-a	2	3					
J004044+404845	00:40:44.26	+40:48:45.70	14.22	AB0437-b	3	4	12.50	31.89			
	00:40:44.29	+40:48:46.59	8.51	AH0221-a	3	4					

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
	00:40:44.38	+40:48:44.76	11.97	AM0464-a	3	4			49.89	6.24	-0.91
	00:40:44.38	+40:48:47.60	15.28	AB0437-a	3	4					
J004055+405722	00:40:55.78	+40:57:22.90	27.88	AC0308-3	4	6	28.09	9.06			
	00:40:55.79	+40:57:22.40	27.53	AB0437-b	4	6					
	00:40:55.87	+40:57:24.30	29.09	AB0437-a	4	6					
	00:40:55.88	+40:57:23.48	25.55	AH0221-a	4	6			149.33	7.59	-1.09
	00:40:55.94	+40:57:23.80	29.02	AM0464-a	4	6					
	00:40:56.08	+40:57:22.70	29.50	AB0491-a	4	6					
J004016+405825	00:40:16.70	+40:58:25.20	22.20	AC0308-3	5	6	21.58	34.98	129.62	4.45	-1.17
	00:40:16.75	+40:58:24.10	24.72	AB0437-b	5	6					
	00:40:16.83	+40:58:26.40	24.14	AB0437-a	5	6					
	00:40:16.91	+40:58:26.10	22.83	AM0464-a	5	6					
	00:40:16.93	+40:58:24.36	14.03	AH0221-a	5	6					
	00:40:17.03	+40:58:24.80	21.55	AB0491-a	5	6					
J004024+410709	00:40:24.53	+41:07:09.50	28.32	AB0437-b	6	5	28.22	6.93			
	00:40:24.55	+41:07:09.60	28.92	AC0308-3	6	5					
	00:40:24.58	+41:07:11.40	30.17	AB0437-a	6	5			82.98	6.03	-0.71
	00:40:24.66	+41:07:11.70	26.97	AM0464-a	6	5					
	00:40:24.78	+41:07:11.30	26.70	AB0491-a	6	5					
J004013+410842	00:40:13.51	+41:08:42.80	42.21	AC0308-3	7	3	41.21	26.55			
	00:40:13.52	+41:08:43.20	51.15	AB0437-a	7	3					
	00:40:13.60	+41:08:44.20	30.27	AB0491-a	7	3					
J004054+411147	00:40:54.62	+41:11:47.20	1.55	AB0437-a	8	3	1.56	3.62			
	00:40:54.64	+41:11:47.62	1.52	AM0464-a	8	3					
	00:40:54.71	+41:11:48.10	1.62	AH0524-a	8	3					
J004129+405059	00:41:29.47	+40:50:59.30	4.39	AB0437-b	9	3	3.01	48.78			
	00:41:29.48	+40:51:01.17	1.54	AM0464-a	9	3					
	00:41:29.59	+40:51:02.40	3.09	AB0437-a	9	3					
J004121+405259	00:41:21.55	+40:52:59.80	4.51	AB0437-b	10	6	3.91	31.20			
	00:41:21.56	+40:53:02.50	4.10	AB0437-a	10	6					
	00:41:21.61	+40:53:00.50	4.73	AM0464-a	10	6			23.22	1.56	-1.17
	00:41:21.62	+40:53:01.90	2.93	AH0221-a	10	6					
	00:41:21.75	+40:53:00.30	4.50	AB0491-a	10	6					
	00:41:21.89	+40:52:59.80	2.69	AC0308-3	10	6					
J004151+405433	00:41:51.54	+40:54:33.00	2.19	AM0464-a	11	2	2.31	5.19	10.29	0.52	-0.98
	00:41:51.55	+40:54:34.30	2.43	AB0437-a	11	2					
J004141+410334	00:41:41.01	+41:03:34.00	49.17	AB0437-a	12	4	48.78	6.53			
	00:41:41.12	+41:03:36.30	51.05	AH0524-a	12	4					
	00:41:41.14	+41:03:34.42	45.59	AH0221-a	12	4					
	00:41:41.14	+41:03:34.40	49.30	AM0464-a	12	4			157.15	6.33	-0.77
J004130+410501	00:41:30.19	+41:05:01.50	2.49	AB0437-a	13	3	2.12	33.12			
	00:41:30.23	+41:05:03.02	1.42	AM0464-a	13	3					
	00:41:30.26	+41:05:03.80	2.46	AH0524-a	13	3					
J004119+411041	00:41:19.59	+41:10:41.10	7.64	AC0308-3	14	6	16.94	54.90			
	00:41:19.62	+41:10:40.90	20.08	AB0437-a	14	6					
	00:41:19.65	+41:10:42.85	16.51	AH0221-a	14	6					
	00:41:19.68	+41:10:41.40	18.22	AM0464-a	14	6					
	00:41:19.74	+41:10:42.90	19.57	AH0524-a	14	6			69.46	3.43	-0.92
	00:41:19.75	+41:10:43.00	19.63	AC0308-1	14	6					
J004100+411352	00:41:00.14	+41:13:52.90	6.53	AB0437-a	15	4	5.73	49.43			
	00:41:00.24	+41:13:52.70	5.95	AM0464-a	15	4					
	00:41:00.26	+41:13:54.40	7.56	AH0524-a	15	4			15.44	0.86	-0.65
	00:41:00.37	+41:13:55.40	2.90	AC0308-3	15	4					
J004150+411436	00:41:50.75	+41:14:36.00	27.74	AC0308-1	16	6	24.13	14.97			
	00:41:50.77	+41:14:35.00	23.04	AB0437-a	16	6					
	00:41:50.87	+41:14:36.70	26.57	AH0524-a	16	6					
	00:41:50.92	+41:14:37.35	21.45	AH0221-a	16	6			134.96	5.10	-1.13
	00:41:50.94	+41:14:35.30	22.38	AM0464-a	16	6					
	00:41:51.02	+41:14:34.00	23.59	AB0491-a	16	6					
J004147+411845	00:41:47.62	+41:18:45.60	43.74	AB0437-a	17	11	39.87	59.49			
	00:41:47.69	+41:18:46.40	50.49	AH0524-a	17	11					
	00:41:47.75	+41:18:45.00	31.13	AM0464-a	17	11					
	00:41:47.82	+41:18:46.50	47.38	AC0308-1	17	11					
	00:41:47.93	+41:18:47.96	30.44	AH0139-a	17	11					
	00:41:47.94	+41:18:47.80	50.82	AC0101-a	17	11					
	00:41:47.98	+41:18:48.60	48.35	AB0551-a	17	11					
	00:41:47.99	+41:18:47.19	16.15	AT0149-a	17	11					
	00:41:48.01	+41:18:46.46	23.96	AH0221-a	17	11					
	00:41:48.02	+41:18:48.20	47.23	AB0679-a	17	11					
	00:41:48.03	+41:18:48.10	48.86	AB0679-b	17	11					
J004111+404606	00:41:11.96	+40:46:06.39	2.03	AB0437-b	18	2	1.59	27.67			
	00:41:12.00	+40:46:07.30	1.15	AB0437-a	18	2					
J003927+405425	00:39:27.00	+40:54:25.70	3.02	AH0221-a	19	2	3.82	20.84	12.72	0.74	-0.79
	00:39:27.05	+40:54:25.00	4.61	AB0437-b	19	2					
J004013+405005	00:40:13.52	+40:50:05.90	49.07	AB0437-b	20	5	39.29	38.30			

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
	00:40:13.55	+40:50:05.70	44.06	AC0308-3	20	5					
	00:40:13.64	+40:50:06.20	38.07	AM0464-a	20	5					
	00:40:13.76	+40:50:05.18	24.24	AH0221-a	20	5					
	00:40:13.84	+40:50:05.90	40.99	AB0491-a	20	5					
J004140+410332	00:41:40.92	+41:03:32.20	48.44	AB0437-b	21	3	40.63	37.06			
	00:41:41.08	+41:03:32.10	25.57	AC0308-3	21	3					
	00:41:41.24	+41:03:32.00	47.87	AB0491-a	21	3					
J004111+403328	00:41:11.43	+40:33:28.70	5.86	AM0464-a	22	2	5.37	9.12			
	00:41:11.55	+40:33:27.80	4.88	AB0491-a	22	2					
J004112+404602	00:41:12.19	+40:46:02.50	1.89	AM0464-a	23	2	1.88	0.27			
	00:41:12.22	+40:46:03.60	1.88	AB0491-a	23	2					
J004152+404643	00:41:52.28	+40:46:43.10	3.60	AM0464-a	24	3	3.65	15.62			
	00:41:52.35	+40:46:42.81	3.13	AH0221-a	24	3					
	00:41:52.46	+40:46:43.30	4.22	AB0491-a	24	3					
J004247+410118*	00:42:47.16	+41:01:18.40	4.09	AB0491-a	25	3	2.87	42.67			
	00:42:47.29	+41:01:18.51	1.99	AB0551-a	25	3					
	00:42:47.38	+41:01:19.50	2.52	AM0464-a	25	3					
J004141+410334	00:41:41.39	+41:03:34.60	41.36	AC0308-1	26	6	40.31	60.61			
	00:41:41.46	+41:03:37.40	44.77	AB0551-a	26	6					
	00:41:41.50	+41:03:38.90	45.71	AB0679-a	26	6					
	00:41:41.51	+41:03:35.74	15.88	AT0149-a	26	6					
	00:41:41.52	+41:03:39.00	47.92	AB0679-b	26	6					
	00:41:41.57	+41:03:37.50	46.25	AC0101-a	26	6					
J004120+411044	00:41:20.12	+41:10:44.70	18.97	AB0551-a	27	3	19.23	2.32			
	00:41:20.17	+41:10:45.10	19.05	AB0679-b	27	3					
	00:41:20.18	+41:10:45.30	19.68	AB0679-a	27	3					
J004100+411356	00:41:00.67	+41:13:56.20	3.77	AC0308-1	28	4	6.07	37.89			
	00:41:00.71	+41:13:58.30	5.53	AB0551-a	28	4					
	00:41:00.81	+41:13:56.90	7.78	AB0679-a	28	4					
	00:41:00.92	+41:13:57.10	7.20	AB0679-b	28	4					
J004151+411439	00:41:51.14	+41:14:39.38	17.68	AH0139-a	29	5	24.36	27.43			
	00:41:51.15	+41:14:36.80	26.79	AC0101-a	29	5					
	00:41:51.17	+41:14:38.60	25.46	AB0551-a	29	5					
	00:41:51.21	+41:14:38.50	25.70	AB0679-a	29	5					
	00:41:51.22	+41:14:38.40	26.19	AB0679-b	29	5					
J004139+413031	00:41:39.52	+41:30:31.90	16.92	AC0308-1	30	4	28.36	40.34			
	00:41:39.54	+41:30:33.00	30.88	AB0551-a	30	4					
	00:41:39.60	+41:30:31.30	32.32	AB0679-a	30	4					
	00:41:39.62	+41:30:31.60	33.32	AB0679-b	30	4					
J004221+410801	00:42:21.98	+41:08:01.36	5.59	AH0221-a	31	6	4.48	44.15	17.48	0.95	-0.89
	00:42:22.02	+41:08:00.70	4.48	AM0464-a	31	6					
	00:42:22.03	+41:08:05.43	2.50	AH0139-a	31	6					
	00:42:22.08	+41:08:03.70	4.86	AB0679-b	31	6					
	00:42:22.09	+41:08:03.80	4.80	AB0679-a	31	6					
	00:42:22.13	+41:08:02.30	4.63	AB0551-a	31	6					
J004203+412637	00:42:03.19	+41:26:37.90	5.85	AB0679-a	32	3	5.58	8.37	27.05	7.05	-1.03
	00:42:03.26	+41:26:39.40	5.11	AB0551-a	32	3					
	00:42:03.29	+41:26:38.10	5.77	AB0679-b	32	3					
J004251+412634	00:42:51.49	+41:26:34.10	19.93	AC0308-1	33	6	24.70	19.32			
	00:42:51.60	+41:26:32.50	26.30	AB0679-a	33	6					
	00:42:51.61	+41:26:32.50	27.03	AB0679-b	33	6					
	00:42:51.63	+41:26:34.58	24.88	AH0221-a	33	6			37.23	1.90	-0.27
	00:42:51.63	+41:26:32.80	25.10	AC0101-a	33	6					
	00:42:51.63	+41:26:33.30	24.97	AB0551-a	33	6					
J004218+412924	00:42:18.83	+41:29:24.30	360.90	AC0101-a	34	5	339.38	16.05			
	00:42:18.85	+41:29:24.00	348.50	AB0679-a	34	5					
	00:42:18.85	+41:29:25.10	346.30	AB0551-a	34	5					
	00:42:18.86	+41:29:24.10	356.30	AB0679-b	34	5					
	00:42:18.94	+41:29:25.00	284.90	AC0308-1	34	5					
J004326+411912	00:43:26.11	+41:19:12.27	3.57	AH0139-a	35	5	4.86	26.57			
	00:43:26.15	+41:19:11.90	4.76	AB0679-a	35	5					
	00:43:26.16	+41:19:11.80	5.09	AB0679-b	35	5					
	00:43:26.25	+41:19:11.40	5.41	AB0551-a	35	5					
	00:43:26.29	+41:19:11.96	5.48	AH0221-a	35	5			7.97	0.62	-0.32
J004336+412022	00:43:36.40	+41:20:22.40	18.52	AC0101-a	36	3	19.93	10.27			
	00:43:36.53	+41:20:21.10	21.98	AB0551-a	36	3					
	00:43:36.62	+41:20:21.40	19.30	AC0308-1	36	3					
J004344+412839	00:43:44.43	+41:28:39.90	23.83	AB0679-a	37	3	23.50	3.80			
	00:43:44.44	+41:28:39.90	24.07	AB0679-b	37	3					
	00:43:44.54	+41:28:41.20	22.61	AB0551-a	37	3					
J004417+411339	00:44:17.88	+41:13:39.60	13.33	AB0679-a	38	3	12.72	10.56			
	00:44:17.94	+41:13:39.60	13.46	AB0679-b	38	3					
	00:44:18.07	+41:13:40.30	11.38	AB0551-a	38	3					
J004423+413042	00:44:23.80	+41:30:42.40	12.22	AB0551-a	39	3	10.63	20.01			
	00:44:23.90	+41:30:43.10	8.50	AB0647-a	39	3					

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
	00:44:24.02	+41:30:44.20	11.16	AB0647-b	39	3					
J004318+411725	00:43:18.05	+41:17:25.20	5.00	AC0101-a	40	3	6.68	31.44			
	00:43:18.14	+41:17:25.70	8.78	AB0551-a	40	3					
	00:43:18.28	+41:17:24.90	6.26	AM0464-a	40	3					
J004510+410925	00:45:10.58	+41:09:25.60	3.89	AB0647-a	41	2	4.95	21.33			
	00:45:10.71	+41:09:25.90	6.00	AB0647-b	41	2					
J004511+411131	00:45:11.56	+41:11:31.90	20.08	AM0464-a	42	3	14.53	38.20			
	00:45:11.60	+41:11:32.10	9.85	AB0647-a	42	3					
	00:45:11.61	+41:11:31.60	13.66	AB0647-b	42	3					
J004418+411341	00:44:18.29	+41:13:41.70	3.95	AB0647-a	43	3	7.92	50.15			
	00:44:18.38	+41:13:40.20	10.55	AM0464-a	43	3					
	00:44:18.52	+41:13:40.10	9.27	AC0308-2	43	3					
J004513+411449	00:45:13.30	+41:14:49.60	15.03	AM0464-a	44	5	15.49	53.84			
	00:45:13.33	+41:14:51.10	8.45	AB0647-a	44	5					
	00:45:13.41	+41:14:50.70	11.17	AB0647-b	44	5					
	00:45:13.43	+41:14:48.90	23.83	AC0308-2	44	5					
	00:45:13.54	+41:14:47.97	18.97	AH0221-a	44	5			60.99	3.13	-0.90
J004426+411526	00:44:26.32	+41:15:26.80	9.98	AM0464-a	45	3	6.59	51.37			
	00:44:26.45	+41:15:26.90	3.78	AB0647-a	45	3			28.58	4.85	-0.96
	00:44:26.56	+41:15:28.00	6.02	AB0647-b	45	3					
J004626+411937	00:46:26.61	+41:19:37.40	11.37	AB0647-b	46	2	10.02	13.53			
	00:46:26.63	+41:19:38.30	8.66	AB0647-a	46	2					
J004337+412024	00:43:37.08	+41:20:24.20	7.81	AB0647-a	47	2	18.47	57.72			
	00:43:37.25	+41:20:24.30	29.13	AM0464-a	47	2					
J004501+412453	00:45:01.75	+41:24:53.30	44.35	AM0464-a	48	3	36.00	26.06			
	00:45:01.89	+41:24:53.80	26.62	AB0647-a	48	3			140.35	9.10	-0.89
	00:45:01.89	+41:24:53.80	37.03	AB0647-b	48	3					
J004251+412638	00:42:51.68	+41:26:38.10	10.03	AB0647-b	49	2	8.46	18.63			
	00:42:51.76	+41:26:39.20	6.88	AB0647-a	49	2					
J004344+412843	00:43:44.72	+41:28:43.60	12.89	AB0647-a	50	4	18.53	31.48			
	00:43:44.74	+41:28:43.35	21.72	AH0221-a	50	4			105.96	4.70	-1.14
	00:43:44.76	+41:28:44.10	15.14	AB0647-b	50	4					
	00:43:44.78	+41:28:43.20	24.36	AM0464-a	50	4					
J004218+412930	00:42:18.89	+41:29:30.10	106.70	AB0647-a	51	2	131.30	18.74			
	00:42:18.89	+41:29:30.60	155.90	AB0647-b	51	2					
J004450+414029	00:44:50.16	+41:40:29.50	4.23	AB0647-a	52	2	5.28	19.89			
	00:44:50.18	+41:40:29.00	6.33	AB0647-b	52	2					
J004436+414512	00:44:36.95	+41:45:12.50	5.75	AB0647-a	53	2	6.81	15.63			
	00:44:37.06	+41:45:13.80	7.88	AB0647-b	53	2					
J004424+415421	00:44:24.66	+41:54:21.70	3.73	AB0647-a	54	2	4.86	23.17	26.01	1.50	-1.10
	00:44:24.74	+41:54:21.50	5.98	AB0647-b	54	2					
J004541+415507	00:45:41.90	+41:55:07.80	3.29	AB0647-a	55	2	3.67	10.35			
	00:45:41.99	+41:55:07.60	4.05	AM0464-a	55	2					
J004359+415716	00:43:59.06	+41:57:16.20	51.53	AB0647-b	56	2	44.92	14.70	438.23	26.92	-1.49
	00:43:59.15	+41:57:16.80	38.32	AB0647-a	56	2					
J004235+415746	00:42:35.75	+41:57:46.20	76.87	AC0496-a	57	4	44.17	74.05	183.44	14.01	-0.93
	00:42:35.77	+41:57:43.40	24.40	AB0647-b	57	4					
	00:42:35.84	+41:57:44.50	16.73	AB0647-a	57	4					
	00:42:35.90	+41:57:46.40	58.66	AC0308-1	57	4					
J004647+420852	00:46:47.64	+42:08:52.00	5.89	AB0647-a	58	2	6.76	12.93			
	00:46:47.69	+42:08:52.30	7.64	AB0647-b	58	2					
J004653+414908	00:46:53.09	+41:49:08.30	2.82	AB0647-b	59	2	5.21	45.93			
	00:46:53.10	+41:49:06.50	7.61	AM0464-a	59	2					
J004509+414956	00:45:09.65	+41:49:56.87	2.04	AB0647-a	60	2	2.62	21.99			
	00:45:09.72	+41:49:58.20	3.19	AB0647-b	60	2					
J004542+415510	00:45:42.01	+41:55:10.47	2.75	AH0221-a	61	2	3.46	20.63			
	00:45:42.05	+41:55:10.60	4.18	AB0647-b	61	2			10.51	0.79	-0.73
J004146+411639	00:41:46.47	+41:16:39.50	5.18	AB0679-a	62	2	4.71	9.86			
	00:41:46.60	+41:16:39.70	4.25	AB0679-b	62	2					
J004108+412454	00:41:08.11	+41:24:54.70	10.76	AB0679-a	63	2	12.15	11.44			
	00:41:08.18	+41:24:55.20	13.54	AB0679-b	63	2					
J004152+412439	00:41:52.30	+41:24:39.70	5.45	AB0679-b	64	2	4.95	10.21			
	00:41:52.38	+41:24:39.80	4.44	AB0679-a	64	2					
J004145+412621	00:41:45.49	+41:26:21.50	6.78	AB0679-a	65	2	6.80	0.29			
	00:41:45.56	+41:26:20.90	6.82	AB0679-b	65	2					
J004247+411525	00:42:47.77	+41:15:25.86	1.10	AH0139-a	66	5	4.26	233.49			
	00:42:47.85	+41:15:27.10	2.51	AB0679-b	66	5					
	00:42:47.86	+41:15:27.40	2.38	AB0679-a	66	5					
	00:42:47.89	+41:15:29.60	14.20	AH0524-a	66	5					
	00:42:47.92	+41:15:28.26	1.10	AH0221-a	66	5					
J004250+411610	00:42:50.34	+41:16:10.40	0.98	AT0149-a	67	5	5.66	101.06			
	00:42:50.36	+41:16:12.20	9.44	AB0679-a	67	5					
	00:42:50.38	+41:16:13.90	11.38	AB0679-b	67	5					
	00:42:50.39	+41:16:10.29	4.26	AH0221-a	67	5			8.26	0.70	-0.25
	00:42:50.40	+41:16:10.67	2.24	AH0139-a	67	5					

Continued on the next page...

Name	RA (J2000)	Dec (J2000)	Flux	Project	GroupID	GroupSize	Average	Error	GFlux	GError Flux	Alpha
	h m s	° ′ ″	(mJy)				(mJy)	(%)	(mJy)	(mJy)	
J004226+411804	00:42:26.61	+41:18:04.83	1.63	AH0221-a	68	3	1.66	1.81	3.65	0.59	-0.52
	00:42:26.71	+41:18:05.10	1.67	AB0679-b	68	3					
	00:42:26.71	+41:18:05.20	1.68	AB0679-a	68	3					
J004248+411945	00:42:48.99	+41:19:45.90	1.31	AB0679-a	69	2	1.37	4.38			
	00:42:49.02	+41:19:46.00	1.43	AB0679-b	69	2					
J004220+412638	00:42:20.56	+41:26:38.60	4.69	AB0679-a	70	2	4.92	4.58			
	00:42:20.57	+41:26:38.50	5.14	AB0679-b	70	2					
J004223+412905	00:42:23.49	+41:29:05.60	4.39	AB0679-b	71	2	2.92	50.09			
	00:42:23.49	+41:29:06.40	1.46	AB0679-a	71	2					
J004317+411723	00:43:17.94	+41:17:23.40	7.63	AB0679-a	72	3	6.18	50.81			
	00:43:17.96	+41:17:23.30	7.87	AB0679-b	72	3					
	00:43:18.00	+41:17:22.58	3.04	AH0221-a	72	3			22.85	0.70	-0.86
J004337+412026	00:43:37.22	+41:20:26.60	31.64	AB0679-a	73	2	31.23	1.33			
	00:43:37.22	+41:20:26.80	30.81	AB0679-b	73	2					
J004338+412648	00:43:38.67	+41:26:48.00	2.27	AB0679-b	74	2	2.19	3.65			
	00:43:38.68	+41:26:48.50	2.11	AB0679-a	74	2					
J004425+411525	00:44:25.91	+41:15:25.80	10.40	AB0679-a	75	2	10.50	0.95			
	00:44:25.93	+41:15:25.70	10.60	AB0679-b	75	2					
J004406+413107	00:44:06.91	+41:31:07.60	5.65	AB0679-b	76	2	4.38	29.00			
	00:44:06.91	+41:31:08.70	3.11	AB0679-a	76	2					
J004354+404636	00:43:54.34	+40:46:36.20	122.30	AC0308-1	77	2	130.10	6.00			
	00:43:54.38	+40:46:34.50	137.90	AH0221-a	77	2			530.96	26.03	-0.92
J004341+405429	00:43:41.03	+40:54:29.83	40.76	AH0221-a	78	2	54.73	25.53			
	00:43:41.10	+40:54:28.90	68.71	AC0308-1	78	2			191.13	7.32	-0.82
J004358+415716	00:43:58.78	+41:57:16.90	104.80	AC0496-a	79	2	104.40	0.38			
	00:43:58.83	+41:57:17.10	104.00	AC0308-1	79	2					
J004611+420408	00:46:11.74	+42:04:08.00	7.61	AC0308-2	80	2	4.95	53.89			
	00:46:11.82	+42:04:07.89	2.28	AB0647-b	80	2					
J004758+420513	00:47:58.94	+42:05:13.00	14.50	AC0308-2	81	2	9.50	52.71			
	00:47:59.10	+42:05:13.54	4.49	AH0221-a	81	2			99.94	5.07	-1.54
J004111+402411	00:41:11.30	+40:24:11.01	11.50	AH0221-a	82	2	12.04	4.45	45.74	2.58	-0.87
	00:41:11.43	+40:24:10.30	12.57	AC0308-3	82	2					
J004030+402756	00:40:30.17	+40:27:56.30	5.20	AC0308-3	83	2	5.41	3.88			
	00:40:30.30	+40:27:55.50	5.62	AM0464-a	83	2			11.79	0.79	-0.51
J003936+403345	00:39:36.61	+40:33:45.50	4.39	AM0464-a	84	2	4.42	0.79			
	00:39:36.71	+40:33:45.90	4.46	AC0308-3	84	2					
J004046+405525	00:40:46.50	+40:55:25.84	1.20	AB0437-b	85	2	2.46	51.12			
	00:40:46.61	+40:55:24.80	3.71	AC0308-3	85	2					
J003935+411432	00:39:35.96	+41:14:32.73	4.74	AH0524-a	86	2	4.35	8.97			
	00:39:36.06	+41:14:33.10	3.96	AC0308-3	86	2					
J003918+410301	00:39:18.49	+41:03:01.03	9.27	AH0524-a	87	2	7.34	26.29			
	00:39:18.55	+41:03:00.50	5.41	AM0464-a	87	2					
J004058+410331	00:40:58.64	+41:03:31.90	1.90	AM0464-a	88	2	2.25	15.74			
	00:40:58.65	+41:03:33.00	2.61	AH0524-a	88	2					
J004035+410453	00:40:35.47	+41:04:53.00	1.41	AM0464-a	89	2	1.39	1.81			
	00:40:35.58	+41:04:53.70	1.36	AH0524-a	89	2					
J004013+410836	00:40:13.58	+41:08:36.80	28.27	AM0464-a	90	2	17.29	63.50			
	00:40:13.69	+41:08:36.59	6.31	AH0221-a	90	2					
J004210+410225	00:42:10.29	+41:02:25.46	1.34	AB0679-b	91	4	1.50	32.44			
	00:42:10.34	+41:02:25.53	1.98	AH0221-a	91	4					
	00:42:10.35	+41:02:24.05	1.05	AB0491-a	91	4					
	00:42:10.48	+41:02:25.00	1.61	AM0464-a	91	4					
J004339+412653*	00:43:39.09	+41:26:53.60	1.03	AB0647-b	92	3	2.57	59.97			
	00:43:39.20	+41:26:53.60	3.44	AH0221-a	92	3			8.07	0.65	-0.75
	00:43:39.32	+41:26:53.80	3.25	AM0464-a	92	3					
J004430+411554	00:44:30.19	+41:15:54.17	2.21	AH0221-a	93	2	2.20	0.68			
	00:44:30.25	+41:15:55.80	2.18	AM0464-a	93	2					
J004205+404920	00:42:05.75	+40:49:20.90	1.47	AH0221-a	94	2	1.63	9.82	4.11	0.48	-0.61
	00:42:05.76	+40:49:22.16	1.79	AB0491-a	94	2					
J004413+411952	00:44:13.29	+41:19:52.63	1.26	AB0679-a	95	2	1.39	9.03			
	00:44:13.30	+41:19:51.26	1.51	AB0551-a	95	2					
J004334+410955	00:43:34.53	+41:09:55.50	2.04	AB0679-a	96	3	2.05	3.25			
	00:43:34.58	+41:09:54.16	2.12	AB0551-a	96	3					
	00:43:34.65	+41:09:55.29	2.00	AB0679-b	96	3					
J004210+410230	00:42:10.63	+41:02:30.14	1.27	AB0679-a	97	2	1.39	8.63			
	00:42:10.66	+41:02:30.32	1.51	AB0551-a	97	2					
J004232+411143	00:42:32.90	+41:11:43.28	1.89	AH0221-a	98	4	1.43	32.40	4.76	0.53	-0.79
	00:42:32.92	+41:11:44.93	0.97	AB0551-a	98	4					
	00:42:32.99	+41:11:45.06	1.38	AB0679-b	98	4					
	00:42:33.01	+41:11:45.24	1.47	AB0679-a	98	4					
J004609+415441	00:46:09.56	+41:54:41.14	1.90	AB0647-a	99	2	3.12	39.20			
	00:46:09.65	+41:54:40.43	4.35	AH0221-a	99	2			8.63	0.68	-0.67
J004318+412421	00:43:18.44	+41:24:21.74	1.06	AB0679-a	100	2	0.98	8.72			
	00:43:18.53	+41:24:21.34	0.89	AB0679-b	100	2					
J004249+412406*	00:42:49.13	+41:24:06.03	1.52	AB0679-a	101	2	1.52	0.33			

Continued on the next page...

Name	RA (J2000) h m s	Dec (J2000) ° ′ ″	Flux (mJy)	Project	GroupID	GroupSize	Average (mJy)	Error (%)	GFlux (mJy)	GError Flux (mJy)	Alpha
	00:42:49.14	+41:24:04.11	1.51	AB0679-b	101	2					
J004309+411859	00:43:09.58	+41:18:59.94	1.22	AB0679-b	102	2	1.16	5.63			
	00:43:09.66	+41:18:59.82	1.09	AB0679-a	102	2					
J004306+411915	00:43:06.58	+41:19:15.02	0.42	AB0679-b	103	2	0.46	9.68			
	00:43:06.64	+41:19:15.09	0.51	AB0679-a	103	2					
J004358+411330*	00:43:58.04	+41:13:30.81	1.06	AB0679-b	104	2	1.25	15.20			
	00:43:58.10	+41:13:30.82	1.44	AB0679-a	104	2					
J004240+411553	00:42:40.27	+41:15:53.48	0.72	AB0679-a	105	2	0.76	4.64			
	00:42:40.29	+41:15:53.14	0.79	AB0679-b	105	2					
J004232+411331	00:42:32.21	+41:13:31.10	0.46	AB0679-a	106	2	0.48	4.17			
	00:42:32.25	+41:13:31.54	0.50	AB0679-b	106	2					
J004247+410127	00:42:47.23	+41:01:27.08	1.63	AB0679-b	107	2	1.77	8.17			
	00:42:47.27	+41:01:26.98	1.92	AB0679-a	107	2					
J004235+412118	00:42:35.00	+41:21:18.04	0.40	AB0679-b	108	2	0.42	3.61			
	00:42:35.17	+41:21:18.16	0.43	AB0679-a	108	2					
J004221+411549	00:42:21.38	+41:15:49.71	0.48	AB0679-b	109	2	0.36	31.51			
	00:42:21.41	+41:15:49.51	0.25	AB0679-a	109	2					

Acknowledgements – We used the KARMA and MIRIAD software packages developed by the ATNF. The National Radio Astronomy Observatory is a facility of the National Science Foundation operated under cooperative agreement by Associated Universities, Inc.

REFERENCES

Blair, W. P., Kirshner, R. P., Chevalier, R. A.: 1981, *Astrophys. J.*, **247**, 879.

Braun, R.: 1990a, *Astrophys. J. Suppl. Ser.*, **72**, 755.

Braun, R.: 1990b, *Astrophys. J. Suppl. Ser.*, **72**, 761.

Braun, R. and Walterbos, R.: 1993, *Astron. Astrophys. Suppl.*, **98**, 327.

Dickel, J. R., Dodorico, S., Felli, M., Dopita, M.: 1982, *Aust. J. of Phys.*, **252**, 582.

Dodorico, S., Dopita, M. A., Benvenuti, P.: 1980, *Astron. Astrophys. Suppl.*, **40**, 67.

Filipović, M. D., Payne, J. L., Reid, W., Danforth, C. W., Staveley-Smith, L., Jones, P. A., White, G. L.: 2005, *Mon. Not. R. Astron. Soc.*, **364**, 217.

Filipović, M. D., Haberl, F., Winkler, P. F., Pietsch, W., Payne, J. L., Crawford, E. J., de Horta, A. Y., Stootman, F. H., Reaser, B. E.: 2008, *Astron. and Astrophys.*, **485**, 63.

Galvin, T. J., Filipović, M. D., Crawford, E. J., Tothill, N. F. H., Wong, G. F., De Horta, A. Y.: 2012, *Serb. Astron. J.*, **184**, 41.

Galvin, T. J., Filipović, M. D., Tothill, N. F. H., Crawford, E. J., O'Brien, A. N., Seymour, N., Pannuti, T. G., Kosakowski, A, R., Sharma, B.: 2014, *Astrophys. Space Sci.*, in press.

O'Brien, Andrew N.; Seymour, Nicholas; Pannuti, Thomas G.; Kosakowski, Alekzander R.; Sharma, Biswas

Gelfand, J. D., Lazio, T. J. W., Gaensler, B. M., 2004, *Astrophys. J. Suppl. Ser.*, **155**, 89.

Gooch, R.: 1996, in "Astronomical Society of the Pacific Conference Series, Vol. 101, Astronomical Data Analysis Software and Systems V", G. H. Jacoby & J. Barnes, ed., 80.

Haberl, F., Sturm, R., Ballet, J., Bomans, D. J., Buckley, D. A. H., Coe, M. J., Corbet, R., Ehle, M., Filipovic, M. D., Gilfanov, M., Hatzidimitriou, D., La Palombara, N., Mereghetti, S., Pietsch, W., Snowden, S., Tiengo, A.: 2012, *Astron. and Astrophys.*, **545**, A128.

Karachentsev, I. D., Karachentseva, V. E., Huchtmeier, W. K., Makarov, D. I.: 2004, *Astron. J.*, **127**, 2031.

Lee, J. H., Lee, M. G.: 2014, *Astron. J.*, **786**, 130.

Magnier, E. A., Prins, S., van Paradijs, J., Lewin, W. H. G., Supper, R., Hasinger, G., Pietsch, W., Truemper, J.: 1995, *Astron. Astrophys. Suppl.*, **114**, 215.

Massey, P., Olsen, K. A. G., Hodge, P. W., Strong, S. B., Jacoby, G. H., Schlingman, W., Smith, R. C.: 2006, *Astron. J.*, **131**, 2478.

Millar, W. C., White, G. L., Filipović, M. D., Payne, J. L., Crawford, E. J., Pannuti, T. G., Staggs, W. D.: 2011, *Astrophys. Space Sci.*, **332**, 221.

Millar, W. C., White, G. L., Filipović, M. D.: 2012, *Serb. Astron. J.*, **184**, 19.

O'Brien, A. N., Filipović, M. D., Crawford, E. J., Tothill, N. F. H., Collier, J. D., De Horta, A. Y., Wong, G. F., Drašković, D., Payne, J. L., Pannuti, T. G., Napier, J. P., Griffith, S. A., Staggs, W. D., Kotuš, S.; 2013, *Astrophys. Space Sci.*, **347**, 159.

Pannuti, T. G., Duric, N., Lacey, C. K., Goss, W. M., Hoopes, C. G., Walterbos, R. A. M., Magnor, M. A.: 2000, *Astrophys. J.*, **544**, 780.

Pannuti, T. G., Schlegel, E. M., Filipović, M. D., Payne, J. L., Petre, R., Harrus, I. M., Staggs, W. D., Lacey, C. K.: 2011, *Astron. J.*, **142**, 20.

Payne, J. L., Filipović, M. D., Pannuti, T. G., Jones, P. A., Duric N., White, G. L., Carpano, S.: 2004a, *Astron. Astrophys.*, **425**, 443.

Payne, J. L., Filipović, M. D., Reid, W., Jones, P. A., Staveley-Smith, L., White, G. L.: 2004, *Mon. Not. R. Astron. Soc.*, **355**, 44.

Payne, J. L., White, G. L., Filipović, M. D., Pannuti, T. G.: 2007, *Mon. Not. R. Astron. Soc.*, **376**, 1793.

Payne, J. L., White, G. L., Filipović, M. D.: 2008, *Mon. Not. R. Astron. Soc.*, **383**, 1175.

Sasaki, M., Pietsch, W., Haberl, F., Hatzidimitriou, D., Stiele, H., Williams, B., Kong, A., Kolb, U.: 2012, *Astron. and Astrophys.*, **544**, A144.

Sault, R. J., Teuben, P. J., Wright, M. C. H.: 1995, in "Astronomical Society of the Pacific Conference Series, Vol. 77, Astronomical Data Analysis Software and Systems IV", R. A. Shaw, H. E. Payne, & J. J. E. Hayes, ed., 433.

20 ЦМ ВЛА РАДИО КОНТИНУМ СТУДИЈА M 31 – СЛИКЕ И КАТАЛОГ ТАЧКАСТИХ ИЗВОРА ДР2: ОСТАТЦИ СУПЕРНОВИХ

T. J. Galvin, M. D. Filipović

University of Western Sydney, Locked Bag 1797, Penrith South DC, NSW 1797, Australia
E–mail: *136525304@student.uws.edu.au, m.filipovic@uws.edu.au*

UDK ...

Представљамо верзију 2 нашег каталога тачкастих радио-извора у галаксији M 31 на λ=20 cm (ν=1.4 GHz). Укупно смо идентификовали 916 дискретних радио-објеката позиционираних у пољу M 31. Упоређивањем нашег каталога са каталогом Gelfand et al. (2004) на λ=92 cm, нашли смо 98 заједничких објеката за које смо израчунали спектралне индексе. Већина (73%) ових објеката има спектралне индексе од α <–0.6, из чега следи да је нетермална емисија доминантна — типично за позадинске галаксије и остатке супернових. Такође, истраживали смо и постајање радио-детекција за 156 познатих остатака супернових детектованих оптичким посматрањимаи и нашли смо 13 таквих објеката. Упоређивања са додатним оптичким, радио и X-зрачним каталозима указују на малу популацију остатака супернових који се могу детектовати на свим овим фреквенцијама.